



## Product catalog **CAMLOG®** Implant System

Valid from August 2020



# Content

## System information

The CAMLOG® Implant System	2
----------------------------	---

## Surgery

Planning	16
PROGRESSIVE-LINE Implants and instruments	19
PROGRESSIVE-LINE Flex instruments	24
PROGRESSIVE-LINE Guide System	28
SCREW-LINE Implants and instruments	34
SCREW-LINE Guide System instruments	40
General surgical instruments	43
Osteotomy set	50
ALTApin set	54
Cover screws	57
Healing caps	57

## Prosthetics

Impression taking	60
Bite registration	61
Fabrication of the plaster model	61
Temporary restoration	62
Esthomic® Abutments	62
CAD/CAM prosthetics	64
CAM titanium blanks	66
Universal abutments	67
Gold-plastic abutment	67
Logfit® Prosthetic system	68
COMFOUR® System	69
Ball abutment anchoring system	73
Locator® Anchoring system	74
Double crown restorations	79
Accessories for abutments	79
Prosthetic instruments	80
Instruments for dental technicians	84
Selection abutments	85

## Auxiliary article

Implants for practice	88
Demonstration models	89
Macro models	89
Literature	90

## Auxiliary information

Indication overview	92
Implant overview	95
Prosthetics overview	96
Screw overview	102
Overview tightening torque	106
Materials	108

## Index

Alphabetical	110
Article number	114
Further documentation	125

# The CAMLOG® Implant System



The CAMLOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, consistent prosthetically oriented Implant system.

All CAMLOG® Products are manufactured with the latest state-of-the-art technology. The CAMLOG® Implant System is continuously being developed by the company's research and development team in collaboration with clinics, universities and dental technicians and therefore stays abreast of the latest technology.

The CAMLOG® and CONELOG® Implant Systems are very well documented scientifically. Studies\* support this with respect to a great many parameters including the Implant surface, time of implantation and/or Implant loading, primary stability, and the connection design. The long-term results of the Promote® Surface are convincing.

The descriptions that follow are not adequate to permit immediate use of the CAMLOG® Implant System.

Instruction by a surgeon experienced in using the system is strongly recommended. CAMLOG® Products should only be used by dentists, doctors, surgeons and dental technicians who have been trained in using the system. Appropriate courses and training sessions are regularly offered by Camlog.

Methodological errors in treatment can result in loss of the Implant and significant loss of peri-Implant bone.

Not all products and services from Camlog are available in all countries.

Packaging units: unless described otherwise, each pack contains one product.

The images in this document are for reference purposes only and may differ from the actual product.

\* see «Further documentation» on page 125

## CAMLOG® PROGRESSIVE-LINE Implants

The new CAMLOG® PROGRESSIVE-LINE Implants make it easier to implement modern treatment concepts such as immediate restorations or immediate loading, which require high primary stability [1, 2]\*.

The geometry of the Implant is consistently designed to develop high initial stability:

- The self-tapping screw Implant has a conically shaped apical area that enables pronounced primary stability even in soft bone [1, 2]\*.
- Thread extending to the apex for good anchorage in immediate implantations [1, 2]\*.
- Crestal thread for improved hold with limited bone height [2]\*.


The CAMLOG® PROGRESSIVE-LINE Implants are available with the Promote® plus surface which features a 0.4 mm high machined Implant neck. Depending on the clinical situation, this surface design thus permits slightly supracrestal or epicrestal Implant positioning.

PROGRESSIVE-LINE Implants with screw-mounted insertion post can be used for the guided implantation.

CAMLOG® PROGRESSIVE-LINE Implants are equipped with the proven Tube-in-Tube® Implant-abutment connection and feature three symmetrically arranged angular grooves in the cylindrical part of the Implant neck. The prosthetic restoration is performed with CAMLOG® Abutments, optionally also with components for Platform Switching.

\* see «Further documentation» on page 125.

### Implant diameters



3.3 mm    3.8 mm    4.3 mm    5.0 mm

### Implant lengths



PROMOTE® PLUS

9 mm    11 mm    13 mm    16 mm



## CAMLOG® SCREW-LINE Implants

CAMLOG® SCREW-LINE Implants are slightly conical, self-tapping screw implants. They enable easy insertion by self-centering with continuous bone contact to achieve solid primary stability.

SCREW-LINE Implants are available with both the Promote® Surface (1.4 mm machined Implant neck section) and the Promote® plus surface (0.4 mm machined Implant neck section) and thus allow maximum flexibility of the vertical Implant position. Rounding of the apical geometry ensures gentle insertion of the SCREW-LINE Implants into the bone, also near the maxillary sinus.

SCREW-LINE Implants with screw-mounted insertion post can be used for the guided implantation.

CAMLOG® SCREW-LINE Implants are equipped with the proven Tube-in-Tube® Implant-abutment connection and feature three symmetrically arranged angular grooves in the cylindrical part of the Implant neck. The prosthetic restoration is performed with CAMLOG® Abutments, optionally also with components for Platform Switching.



### Implant diameters



3.3 mm    3.8 mm    4.3 mm    5.0 mm    6.0 mm

### Implant lengths



9 mm    11 mm    13 mm    16 mm

All CAMLOG® Implants are delivered pre-assembled in sterile packaging on a color-coded insertion post corresponding to the diameter.

The option of Platform Switching may only be used with CAMLOG® Implants with K article numbers.

## CAMLOG® Tube-in-Tube® Implant-abutment connection

The unmistakable Tube-in-Tube principle with the three interlocking grooves and cams creates a very precise, stable, and antirotational implant-abutment connection. This was designed biomechanically on the basis of complex finite element analyses. It has proven itself millions of times over for many years and its long-term success has been scientifically documented.

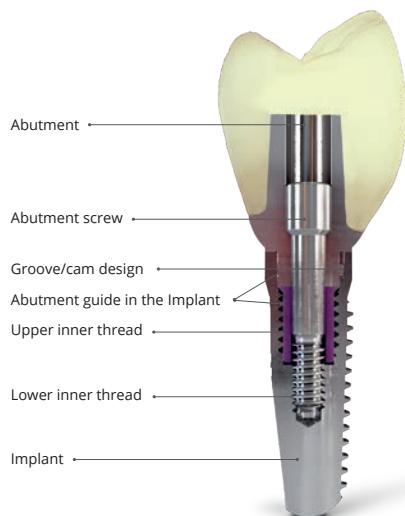
The CAMLOG® Tube-in-Tube® Connection has undergone extensive scientific studies and achieved above average good results for precision fit [3, 4]\*.

\* See «Further documentation» on page 125.

### Advantages and benefits of the Tube-in-Tube® Connection

- Easy indexing thanks to three possible positions of the abutments
- Precise with excellent tactile feedback
- Platform Matching and optional Platform Switching
- Defined vertical stop: no height offset over the entire workflow
- Reduced diameter implant ( $\varnothing$  3.3 mm)
- Scientifically documented long-term results

For optimal positioning of the abutments, the Implant should be aligned in the bone so that one of the three grooves points in vestibular direction. With the CAMLOG® Implants, the insertion tools include markings that correspond to the three grooves of the Implant inner configuration.



### Promote® Surface

CAMLOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface. The surface is based on current scientific knowledge and supports rapid osseointegration. Scientific results from studies with cell cultures, osteohistology and in pull-out trials illustrate this impressively.



### Production precision

The inner and outer geometry of the CAMLOG® Implants and abutments are rotary machined for the most part. The tolerances can therefore be kept very low. The result is excellent part precision without impacting the material structure. The Tube-in-Tube® Implant-abutment connection thus ensures a very precise, stable and rotation-locked connection to the prosthetic components.

## CAMLOG® Prosthetic components

The CAMLOG® Implants can be provided with a wide range of flexible, anatomically adapted prosthetic components. CAMLOG® Abutments are color-coded according to the Implant diameters.

### Effect of the Platform Switching design

Platform Switching is used to support the hard and soft tissue in the peri-Implant esthetic region. The distance between the Implant-abutment interface and the alveolar crest is increased and thereby reduces the effect of inflammatory cell infiltration with concomitant bone resorption. The option of Platform Switching may only be used with CAMLOG® Implants with K article numbers.

### CAMLOG® Healing caps PS for Platform Switching

The CAMLOG® Healing caps PS (cylindrical, wide body, bottleneck) are tapered in diameter at the shoulder support making it possible to adapt soft tissue over the Implant shoulder.



### CAMLOG® Impression posts PS, open and closed tray for Platform Switching

Due to the adaptation of the soft tissue over the Implant shoulder, the use of the CAMLOG® Healing caps PS necessitates the use of the CAMLOG® Impression post PS for Platform Switching.


### CAMLOG® Temporary abutments PS, CAMLOG® Esthetic® Abutments PS, CAMLOG® Titanium base CAD/CAM PS and CAMLOG® Universal abutments PS for Platform Switching

The CAMLOG® Abutments PS are also tapered in diameter in the area of the shoulder support and thus allow adapting soft tissue over the Implant shoulder during prosthetic restoration.





Short cam geometry



## CAMLOG® Abutments with K article numbers

The abutments are extended apically in tubular shape (5.4 mm) and include three short cams in the upper section that correspond to the three grooves in the Implant.

When inserting the abutments, their tubular extension towards the apex affects the simple, easy and safe orientation in the longitudinal axis of the Implant before the three cams lock into the grooves of the Implant shoulder. The abutment is rotated until tactile engagement of the cams in the grooves of the Implant. The abutment is then in the final position.

The Implant-abutment connection of the CAMLOG® Implant System is predominantly a form-fitting connection. The connection with the cam geometry was optimally designed in terms of biomechanics by applying elaborate finite element analyses. The image displays the distribution of the von Mises tension in the Implant-abutment connection in accordance with ISO 14801 at a load of 200 N.

## CAMLOG® Healing caps

The various healing caps are used according to indication for single and two-stage procedures. The CAMLOG® Healing caps are available in three geometries (cylindrical, wide body and bottleneck), both for the standard connections as well as for the Platform Switching option (PS). They are not rotation-locked and are screw-retained in the upper inner thread of the Implants.



## CAMLOG® Impression taking

Impression-taking of the CAMLOG® Implants is possible with impression posts, open or closed tray. Impression posts for Platform Switching (PS) are also an option. All impression-taking components are color-coded based on the Implant diameter. High-precision components ensure correct transfer of the intraoral situation. The antirotational mechanism is ensured by the CAMLOG® groove/cam geometry.



### CAMLOG® Temporary abutments

Various abutments are available for the CAMLOG® Implant System for temporary prosthetic restorations. CAMLOG® Temporary abutments made of titanium alloy (Ti6Al4V ELI) are available in crown and bridge versions.

As an option, temporary restoration on CAMLOG® Implants can also be performed with temporary abutments made of PEEK (poly ether ether ketone). Also as option for Platform Switching (PS). The abutments can be used in immediate implantations or after exposing the gingiva.

### CAMLOG® Titanium bases CAD/CAM

CAMLOG® Titanium bases CAD/CAM are acting as a bonding basis for customized, implant-supported dental restorations made of suitable materials. Reconstructions are fabricated with the aid of CAD/CAM techniques. CAMLOG® Titanium bases CAD/CAM are available in crown and bridge versions.

Optionally a Titanium base CAD/CAM crown PS is also available for Platform Switching.

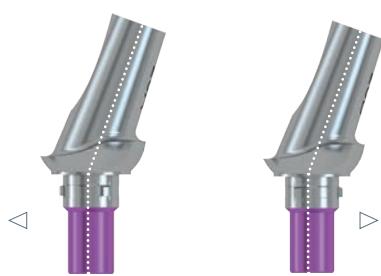


### CAMLOG® Esthomic® Abutments

Anatomically preformed abutments allow for optimal stump design. The CAMLOG® Esthomic® Abutments are available both straight and angled with various gingival heights and with an oval anatomically pre-shaped shoulder profile. The angled Esthomic® Abutments are available in A and B versions differentiated by a cam offset of 60°. This results in six prosthetic-oriented rotating positions and allows perfect prosthetic alignment of the axes.




### CAMLOG® Esthomic® Abutment cam alignment



**Type A**  
Cam alignment  
against the angle

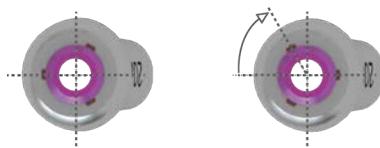**Type B**  
Cam alignment in  
direction of the angle



**Type A**

**Type B**  
Cams with 60° offset



### CAMLOG® Gold-plastic abutment

The CAMLOG® Gold-plastic abutment can be used with the cast-on technique to fabricate a multitude of customized Implant restorations, such as single crowns, mesostructures for cementable bridge restorations and primary abutments for bridging Implant axis divergences in the double crown technique.



### CAMLOG® Logfit® Abutments

The CAMLOG® Logfit® Prosthetic System enables the fabrication of cementable crown and bridge restorations. The Logfit® Prosthetic System consists of prefabricated components precisely matched to one another and thus standardizes the clinical and technical procedure. The result is a lower workload for the practice and the dental laboratory.



### CAMLOG® Universal and telescope abutments

CAMLOG® Universal and telescope abutments can be used for individually fabricated cementable crown and bridge restorations and for double crown restorations. The universal abutment is also available for optional Platform Switching (PS). The abutments are made of titanium alloy and can be custom trimmed.

### CAMLOG® Ball, Locator® and straight bar abutments

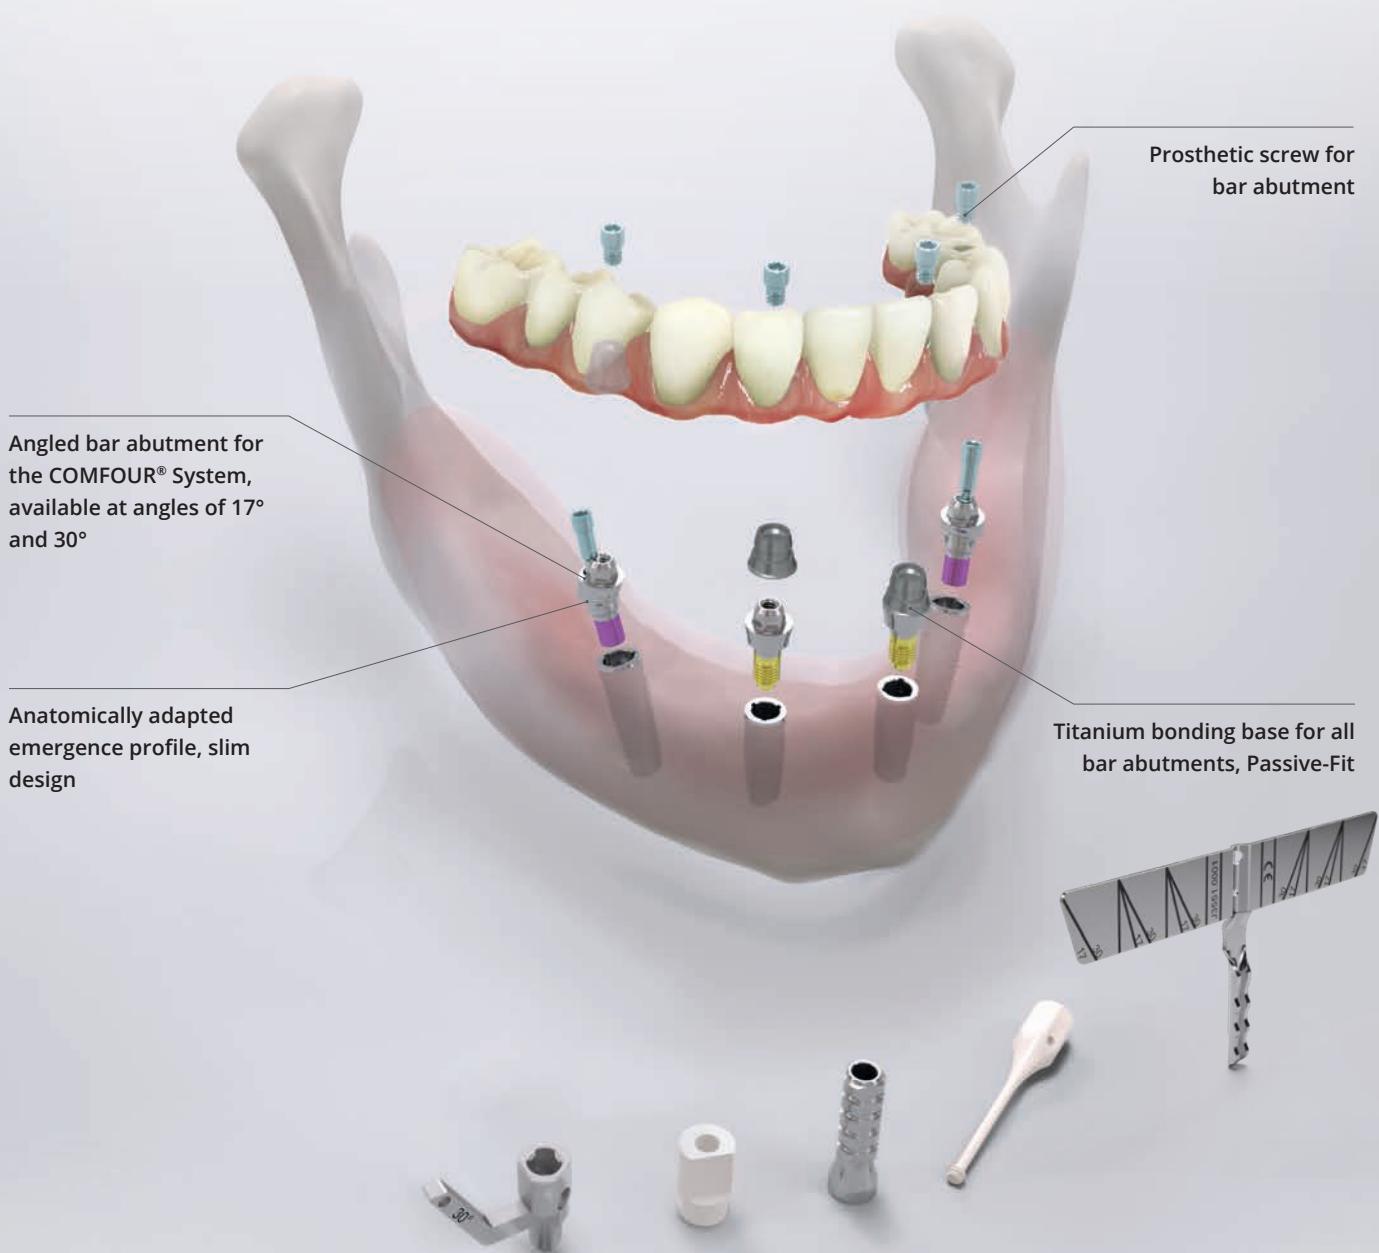
Ball, Locator® and straight bar abutments are available for the CAMLOG® Implant System. These differ from the abutments with abutment screws in the apical region through different connection designs. Ball, Locator® and straight bar abutments are manufactured as single pieces with a thread in the apical region which engages with the upper inner thread of the CAMLOG® Implant. These abutments are screwed into the CAMLOG® Implant using the corresponding insertion tools.



## COMFOUR® System

Occlusally screw-retained restorations are state-of-the-art. With the COMFOUR® System, edentulous patients are given the option of immediate, comfortable and permanent dentures based on four or six Implants as a rule – and thus a considerable gain in quality of life. But clinicians too can look forward to considerably greater comfort and freedom. COMFOUR® offers several treatment concepts. In addition to occlusally screw-retained crowns and bridges for immediate and delayed restorations, the multi-optional system also permits bar restorations on straight and angled bar abutments.

COMFOUR® offers a wide range of options to master the challenges in practice routine easier and with less time in future. Next to its versatility, the COMFOUR® Prosthetic system excels through its slim design in particular. All components are of delicate and low design, which simplifies prosthetic restorations considerably for dentists and dental technicians. In addition, a number of technical highlights ensure that COMFOUR® is not simply just a name, but also a program – for users and patients alike.



COMFOUR® offers a large selection of options to manage the requirements of your practice. Easier and more time-saving.

## Digital service

Individually CAD/CAM fabricated prosthetics, scanning and design services, 3D Implant planning, printed drilling templates and jaw models are available from Camlog through our DEDICAM® Service Division. Personal support with the accustomed competence of our employees as well as processes optimized right down to the finest detail ensure a high degree of certainty of results with the greatest possible individual freedom. Extensive libraries for the open CAD systems from 3Shape, exocad and Dental Wings are available for Implant-supported restorations. Discover your options and start your digital future with DEDICAM®.

DEDICAM® Services are not available in all countries. Please ask your local Camlog representative for details.



# DEDICAM® DIGITAL CONCEPTS

## Color coding of the surgical and prosthetic CAMLOG® Products



## Explanation of symbols

	CE-label
	Consult instructions for use
	Caution, observe the warning notices
	Medical device
	Article number
	Lot number
	Sterilized using irradiation
	Single sterile barrier system with protective packaging outside
	Non-sterile
	Date of manufacture
	Use-by date
	Do not resterilize
	Do not reuse
	Do not use if package is damaged
	Keep away from sunlight
	Temperature limit
	Manufacturer
	MR-Conditional
	Caution: US Federal law restricts this device to sale by or on the order of a dentist or physician.

## Explanation of abbreviations

	Diameter
	Apical diameter
	Gingival diameter
	Prosthetic platform diameter
	Length
	Gingival height
	Poly ether ether ketone
	Polyoxymethylene
	Platform Switching
	Polyphenylsulfone

## General safety instructions and warnings

The descriptions in this product catalog are not sufficient to allow immediate use of the CAMLOG® Implant System. Instruction by a surgeon experienced in using the CAMLOG® Implant System is strongly recommended.

## Packaging PROGRESSIVE-LINE Implants

### Secondary packaging

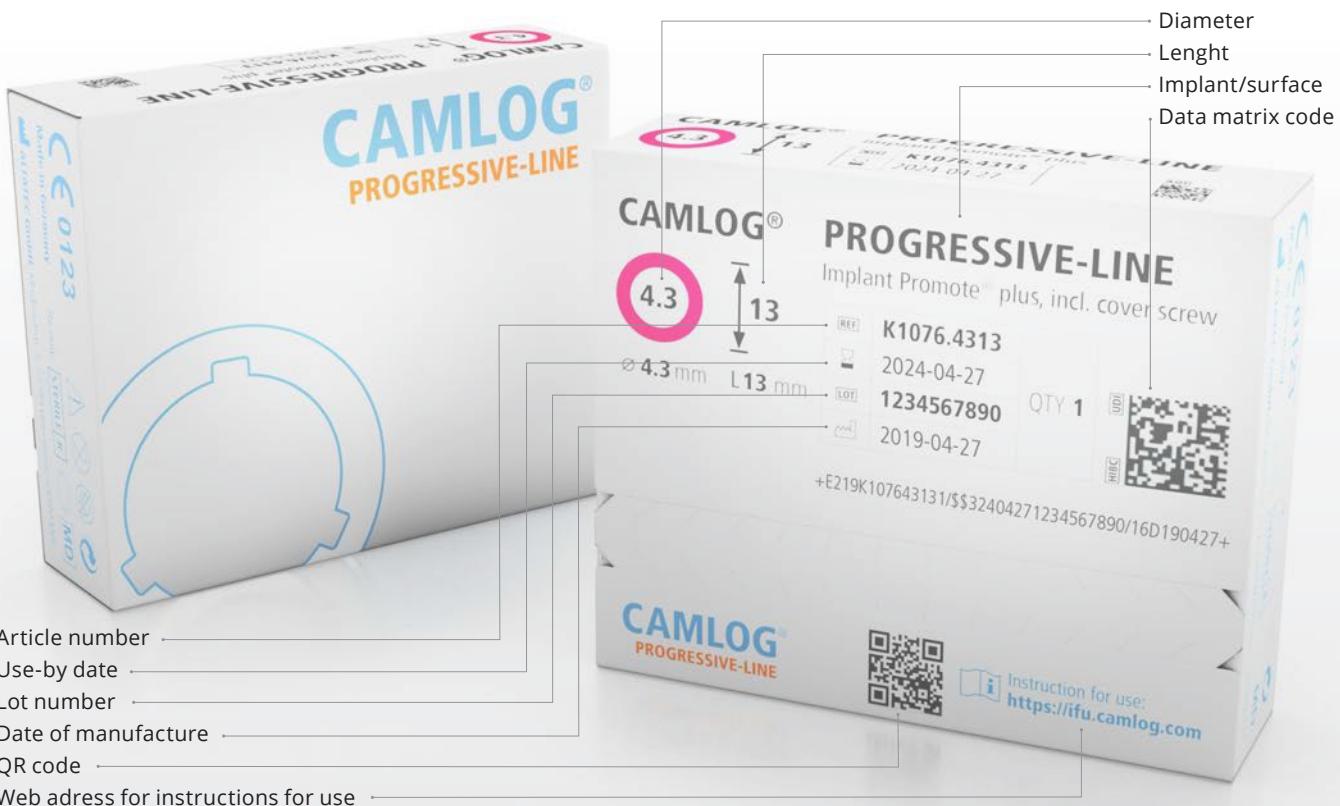
Sealed, folding box with color-coded product label

### Inner Implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer Implant packaging



## Packaging SCREW-LINE Implants

### Secondary packaging

Sealed, folding box with color-coded product label

### Inner Implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer Implant packaging

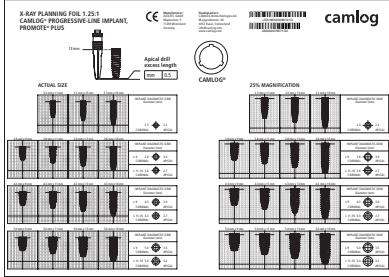
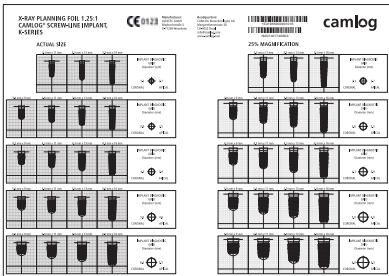
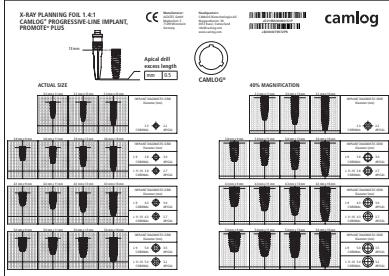
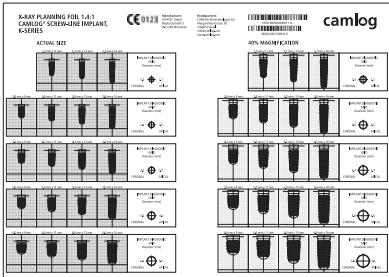
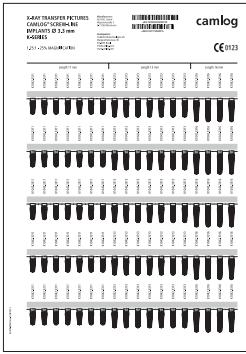






# Planning

## X-Ray Planning foils and X-Ray Transfer pictures

	Article	Art. No.	$\emptyset$
	X-Ray Planning foil 1.25:1 CAMLOG® PROGRESSIVE-LINE Implants Magnification 25%	K5300.9014	-
	X-Ray Planning foil 1.25:1 CAMLOG® SCREW-LINE Implants Magnification 25%	K5300.9010	-
	X-Ray Planning foil 1.4:1 CAMLOG® PROGRESSIVE-LINE Implants Magnification 40%	K5300.9015	-
	X-Ray Planning foil 1.4:1 CAMLOG® SCREW-LINE Implants Magnification 40%	K5300.9011	-
	X-Ray Transfer pictures 1.25:1 CAMLOG® SCREW-LINE Implants Planning foils, self-adhesive Magnification 25%	K5300.9080 K5300.9081 K5300.9082 K5300.9083 K5300.9084	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm

# CT-Planning

For 3-D X-Ray Planning and drilling template

	Article	Art. No.	L
	<b>CT-tube</b> for drill Ø 2.0 mm*, corrugated tubing pack of 10 internal diameter 2.1 mm external diameter 2.5 mm  <b>Material</b> Titanium alloy	A2002.2000	4.0 mm 10.0 mm
	<b>CT-tube</b> for drill Ø 2.2 mm, corrugated tubing pack of 10 internal diameter 2.3 mm external diameter 2.7 mm  <b>Material</b> Titanium alloy	A2222.2200	4.0 mm 10.0 mm
	<b>Drill for CT-tube</b> (for A2002.2000) Ø 2.6 mm  <b>Material</b> Stainless steel	A2050.2600	-
	<b>Drill for CT-tube</b> (for A2222.2200) Ø 2.8 mm  <b>Material</b> Stainless steel	A2050.2800	-

\* for pilot drills J5051.2003 and pilot drills SCREW-LINE J5051.2000



# PROGRESSIVE-LINE

## Implants with snap-in insertion post

Article	Art. No.	$\emptyset$	L	A $\emptyset$
 <p><b>CAMLOG® PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile</b></p> <p><b>Material</b> Titanium Grade 4</p>	K1076.3311	3.3 mm	11 mm	2.2 mm
	K1076.3313		13 mm	
	K1076.3316		16 mm	
	K1076.3809	3.8 mm	9 mm	3.0 mm
	K1076.3811		11 mm	2.7 mm
	K1076.3813		13 mm	
	K1076.3816		16 mm	
	K1076.4309	4.3 mm	9 mm	3.0 mm
	K1076.4311		11 mm	2.7 mm
	K1076.4313		13 mm	
	K1076.4316		16 mm	
	K1076.5009	5.0 mm	9 mm	3.5 mm
	K1076.5011		11 mm	3.2 mm
	K1076.5013		13 mm	
	K1076.5016		16 mm	

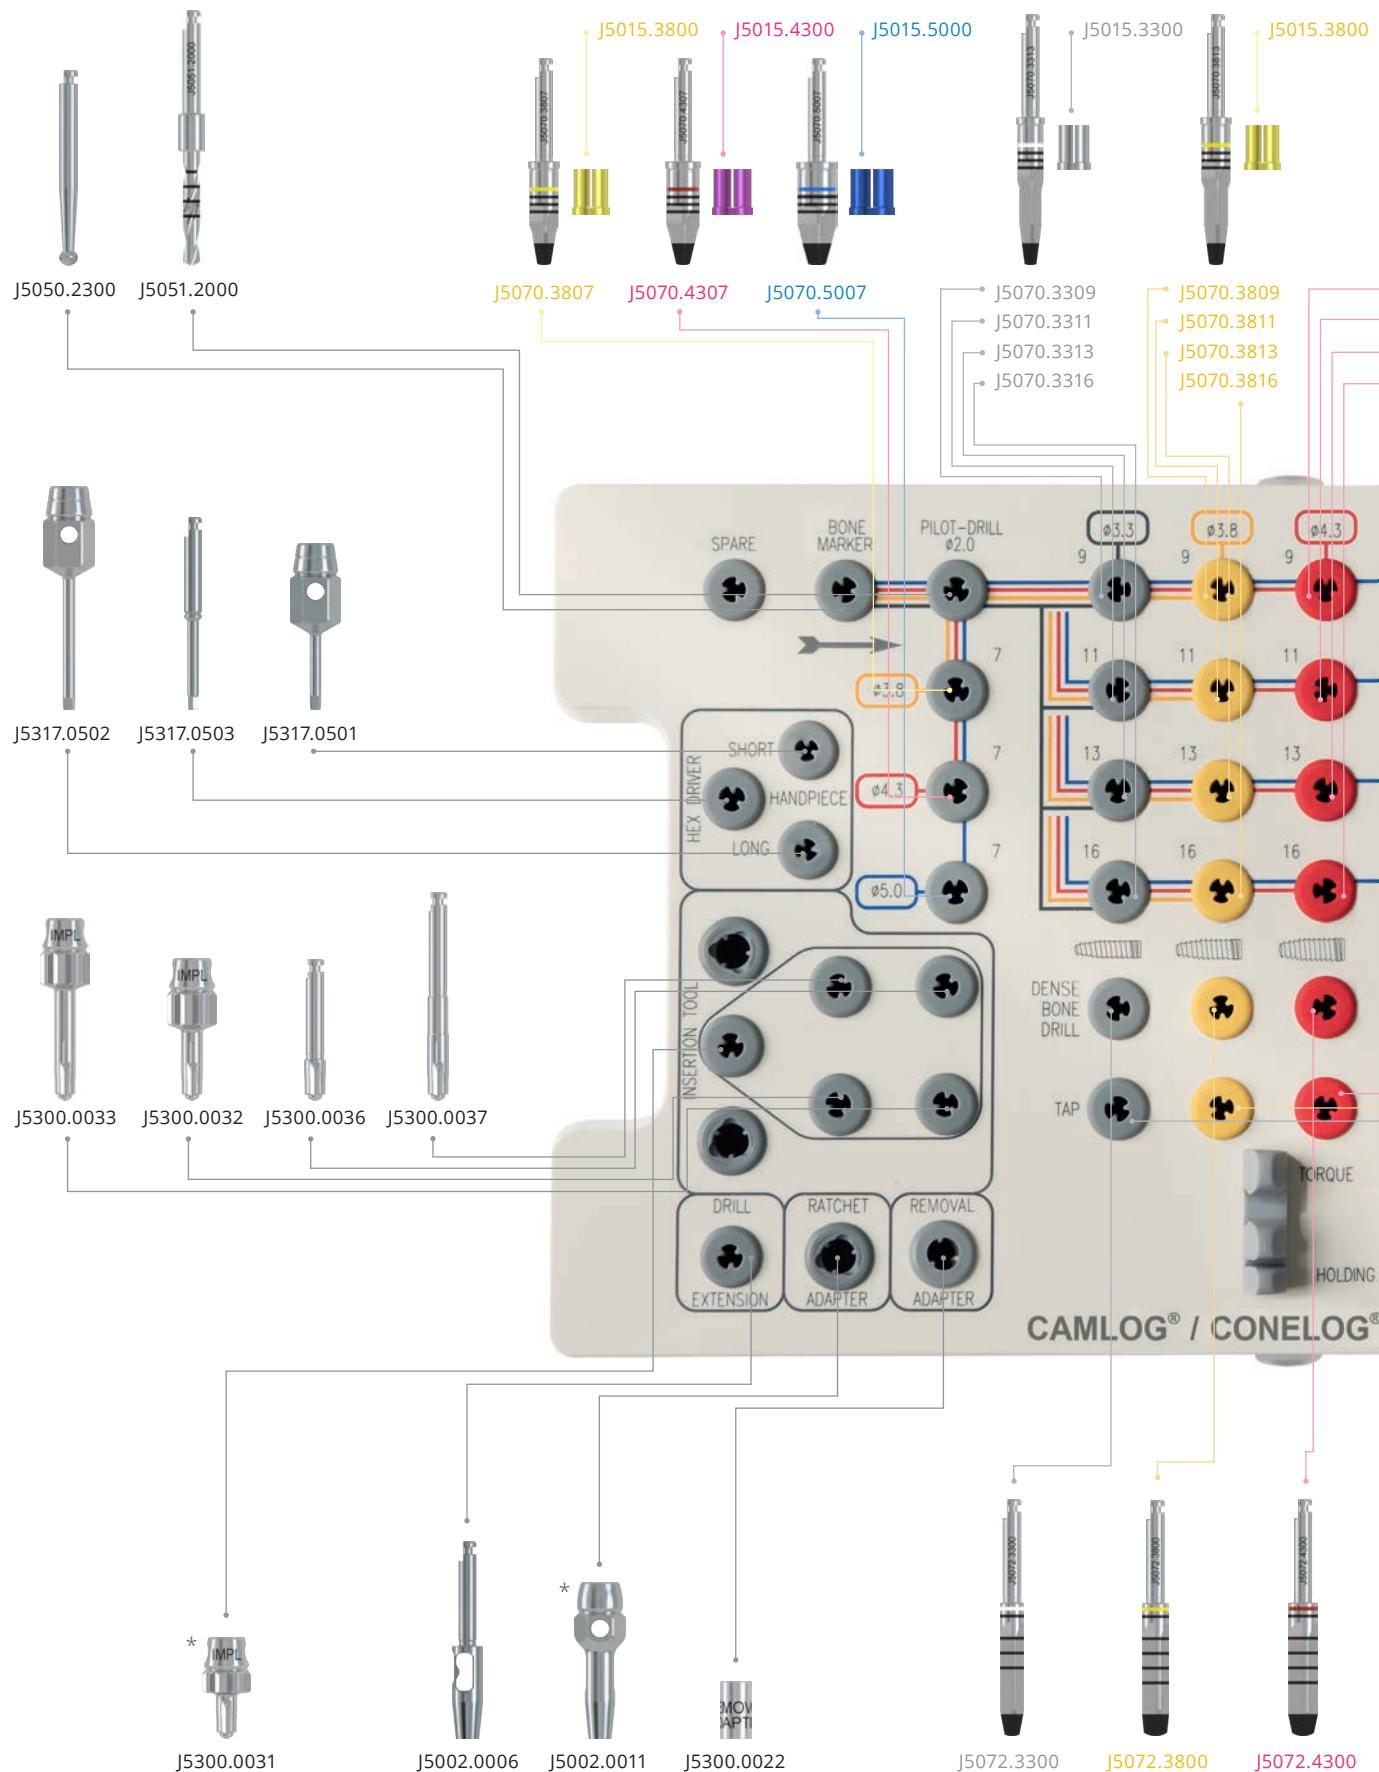
## Implants with screw-mounted insertion post

Article	Art. No.	$\emptyset$	L	A $\emptyset$
 <p><b>CAMLOG® PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile</b></p> <p><b>Material</b> Titanium Grade 4</p>	K1075.3311	3.3 mm	11 mm	2.2 mm
	K1075.3313		13 mm	
	K1075.3316		16 mm	
	K1075.3809	3.8 mm	9 mm	3.0 mm
	K1075.3811		11 mm	2.7 mm
	K1075.3813		13 mm	
	K1075.3816		16 mm	
	K1075.4309	4.3 mm	9 mm	3.0 mm
	K1075.4311		11 mm	2.7 mm
	K1075.4313		13 mm	
	K1075.4316		16 mm	
	K1075.5009	5.0 mm	9 mm	3.5 mm
	K1075.5011		11 mm	3.2 mm
	K1075.5013		13 mm	
	K1075.5016		16 mm	

With CAMLOG® PROGRESSIVE-LINE Implants with the diameters 3.8/4.3/5.0 mm, the option of Platform Switching is possible.

# PROGRESSIVE-LINE

## Surgery set CAMLOG®/CONELOG®




\* These articles are not included in the surgery set and must be ordered separately.

**CAMLOG®**  
PROGRESSIVE-LINE


**CONELOG®**  
PROGRESSIVE-LINE



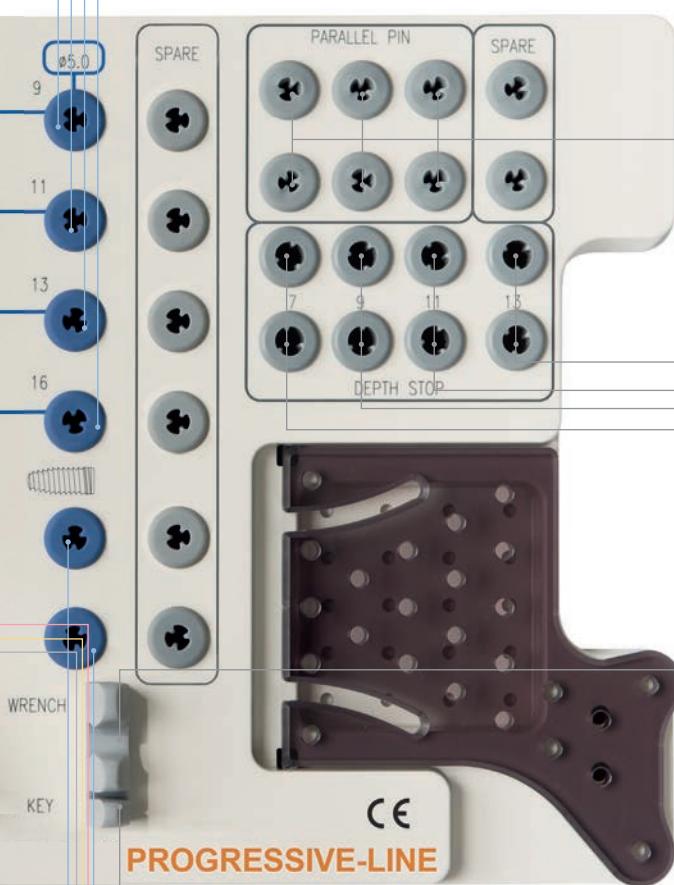- J5070.4309
- J5070.4311
- J5070.4313
- J5070.4316



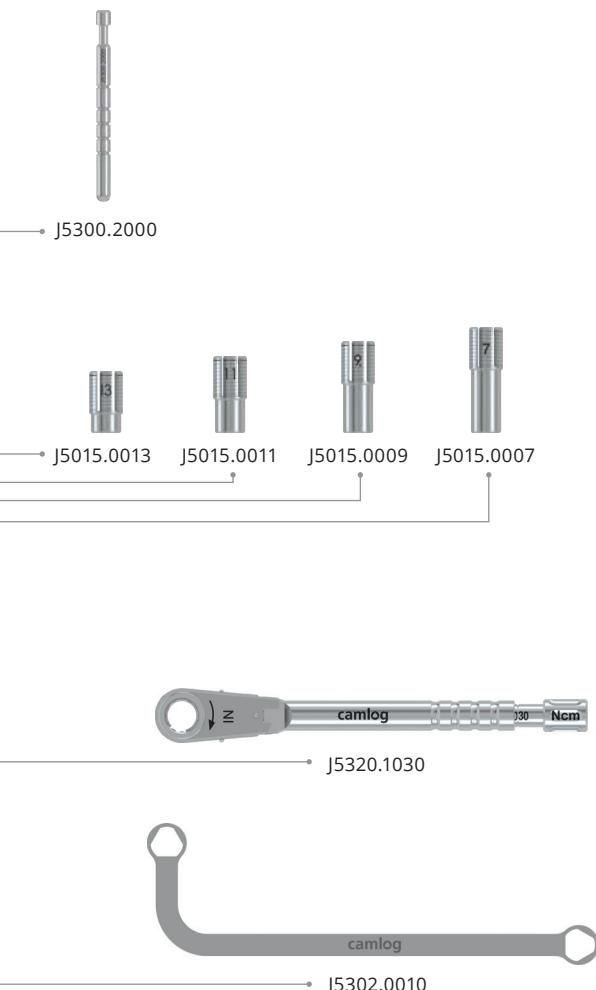The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.



J5072.5000



J5071.3300



J5071.3800





J5071.4300



J5071.5000

# PROGRESSIVE-LINE
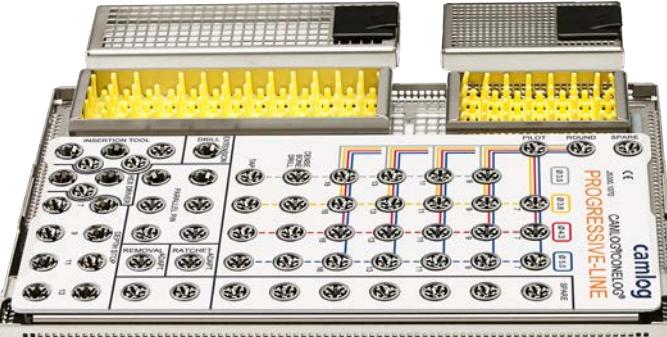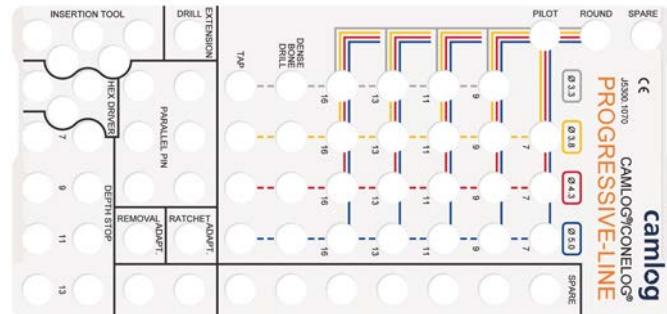
## Surgery set

Article	Art. No.
 <p><b>Surgery set</b>  <b>CAMLOG®/CONELOG® PROGRESSIVE-LINE</b>  contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post (taps are not included)</p>	J5300.0065
 <p><b>Surgery tray</b>  <b>CAMLOG®/CONELOG® PROGRESSIVE-LINE</b>  without content</p>	J5300.8917
 <p><b>Surgery wash tray</b>  <b>CAMLOG®/CONELOG® PROGRESSIVE-LINE</b>  incl. pattern, without content</p>	J5300.8970
 <p><b>Pattern for surgery wash tray</b>  <b>CAMLOG®/CONELOG® PROGRESSIVE-LINE</b>  Material  PPSU</p>	J5300.1070

Preparation of the Implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

## Surgical instruments

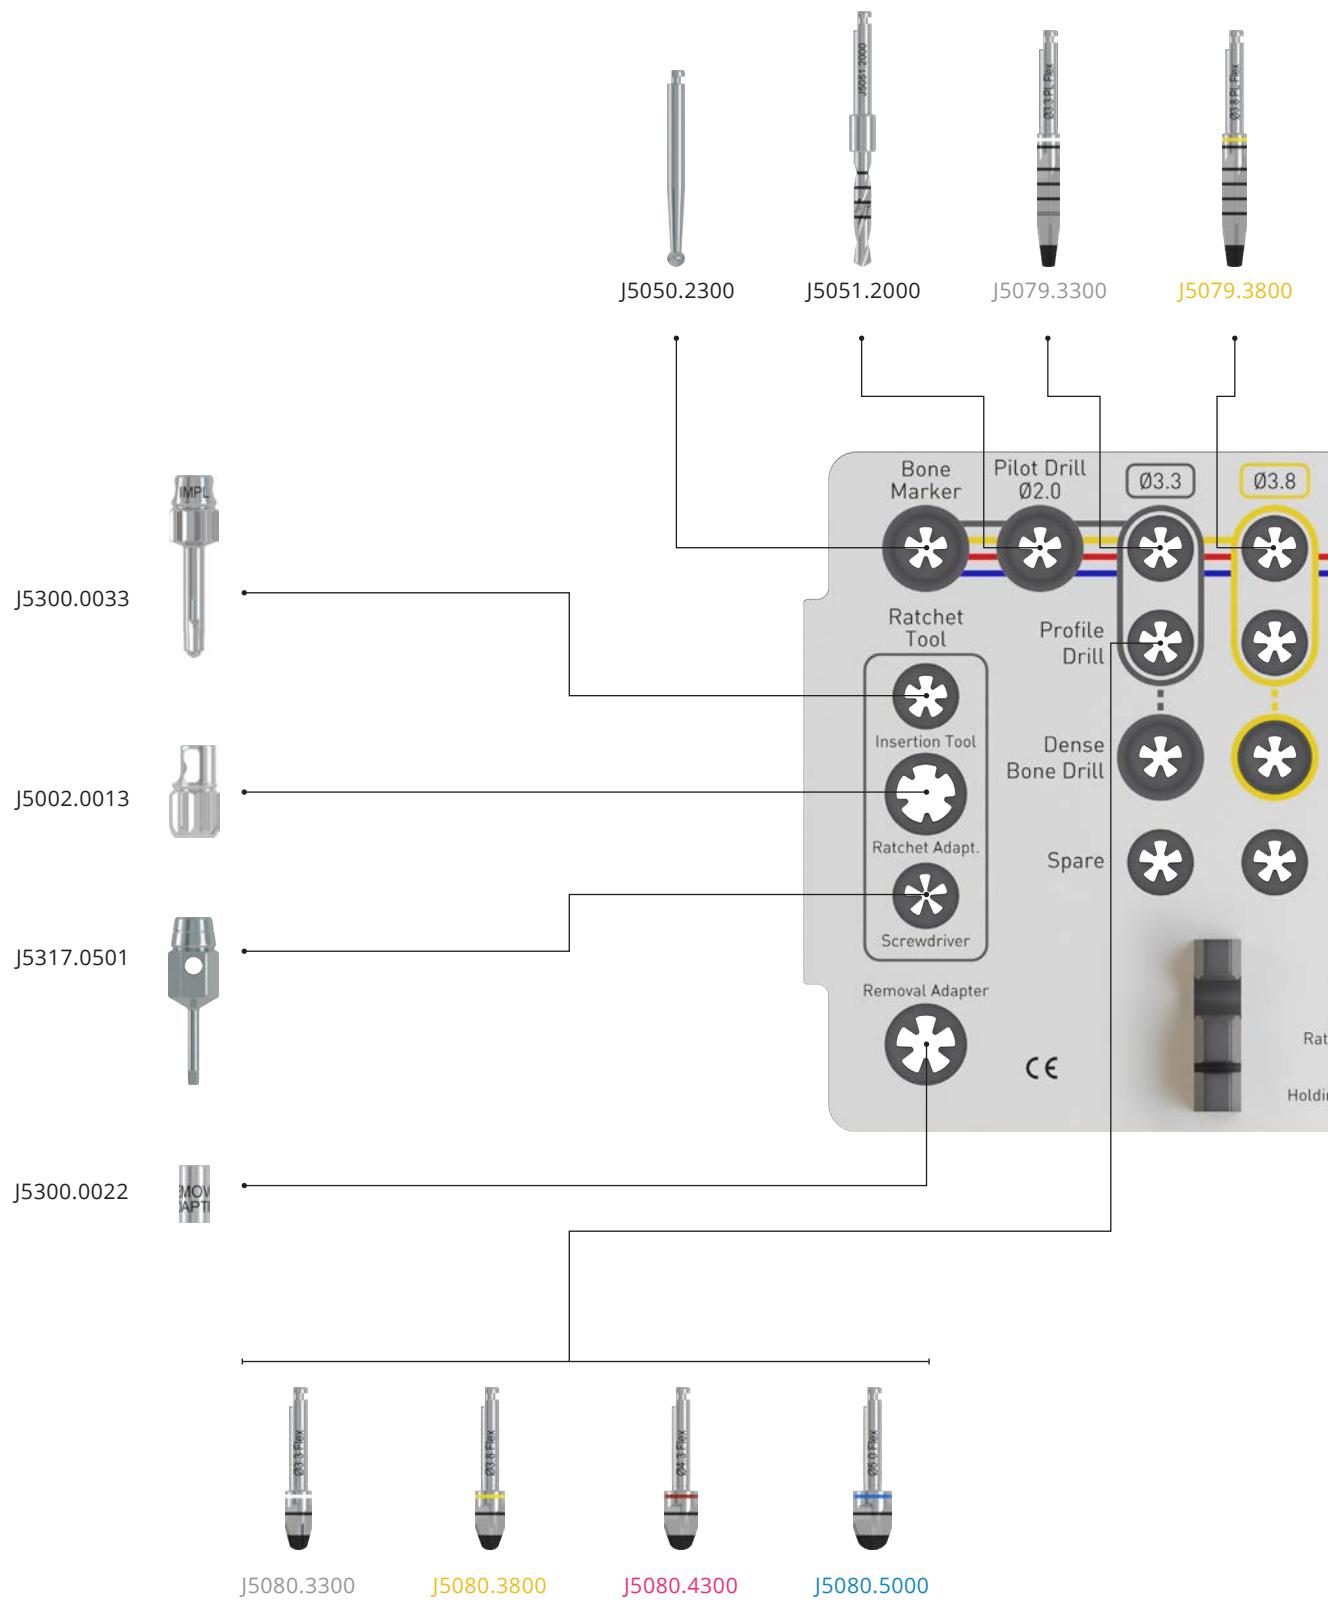
	Article	Art. No.	$\varnothing$	L
	<b>Form drill PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5070.3309	3.3 mm	9 mm
		J5070.3311		11 mm
		J5070.3313		13 mm
		J5070.3316		16 mm
		J5070.3809	3.8 mm	9 mm
		J5070.3811		11 mm
		J5070.3813		13 mm
		J5070.3816		16 mm
		J5070.4309	4.3 mm	9 mm
		J5070.4311		11 mm
		J5070.4313		13 mm
		J5070.4316		16 mm
		J5070.5009	5.0 mm	9 mm
		J5070.5011		11 mm
		J5070.5013		13 mm
		J5070.5016		16 mm
	<b>Depth stop for form drills</b> <b>PROGRESSIVE-LINE and SCREW-LINE</b> resterilizable  <b>Material</b> Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	-
		J5015.4300	4.3 mm	-
		J5015.5000	5.0 mm	-
	<b>Dense bone drill</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	-
		J5072.4300	4.3 mm	-
		J5072.5000	5.0 mm	-
	<b>Tap</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	-
		J5071.4300	4.3 mm	-
		J5071.5000	5.0 mm	-
	<b>Removal adapter for CAMLOG® and CONELOG®</b> suitable for all Implant diameters  <b>Material</b> Stainless steel	J5300.0022*	3.3 mm	6.2 mm
			3.8 mm	
			4.3 mm	
			5.0 mm	
	<b>Paralleling pin</b> <b>PROGRESSIVE-LINE</b> with depth marks (for pilot drilling Ø 2.0 mm)  <b>Material</b> Titanium alloy	J5300.2000	-	-

\* only for use with PROGRESSIVE-LINE Implants with snap-in insertion post

# PROGRESSIVE-LINE Flex


## Surgery set CAMLOG®/CONELOG®

NEW




\* Optional articles, can be purchased separately


**CAMLOG®**  
PROGRESSIVE-LINE



**CONELOG®**  
PROGRESSIVE-LINE



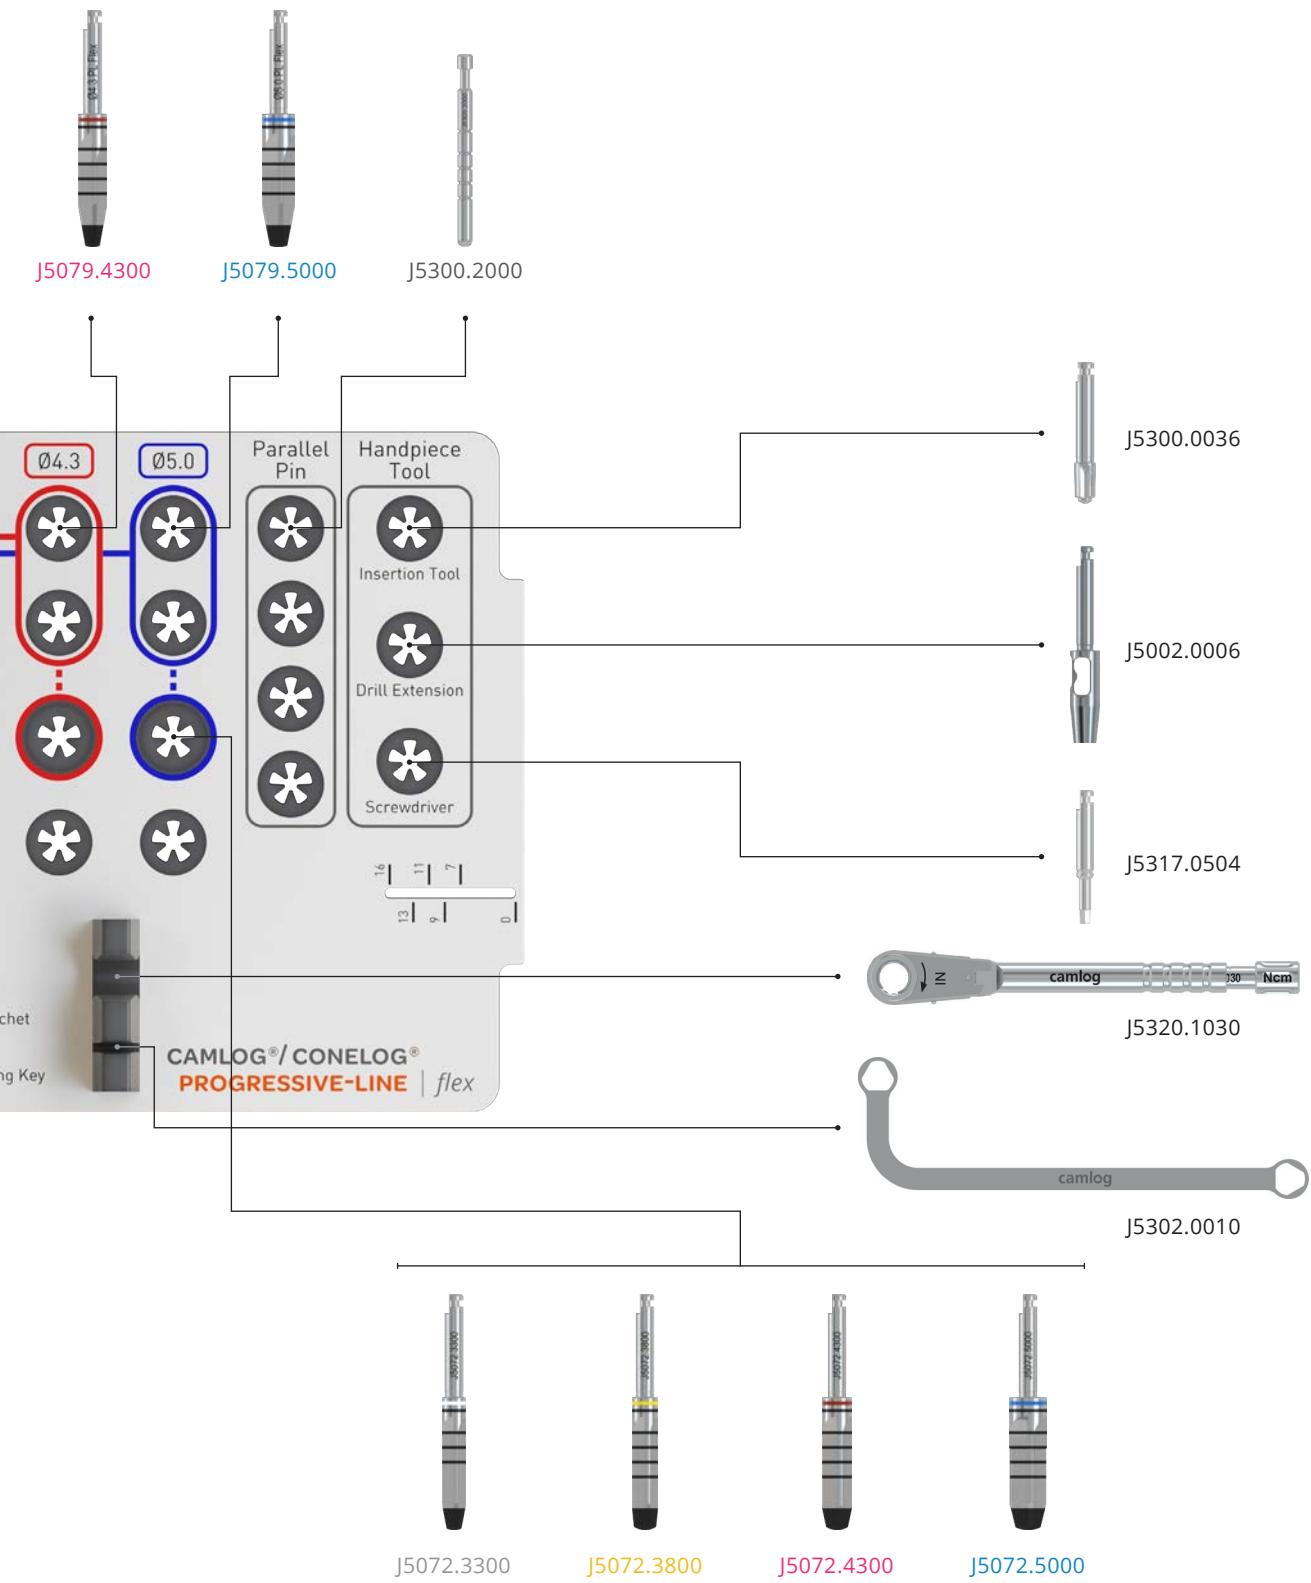The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.



# PROGRESSIVE-LINE Flex

## Surgery set

Article	Art. No.
	J5300.0071
	J5300.8920

## Surgical instruments

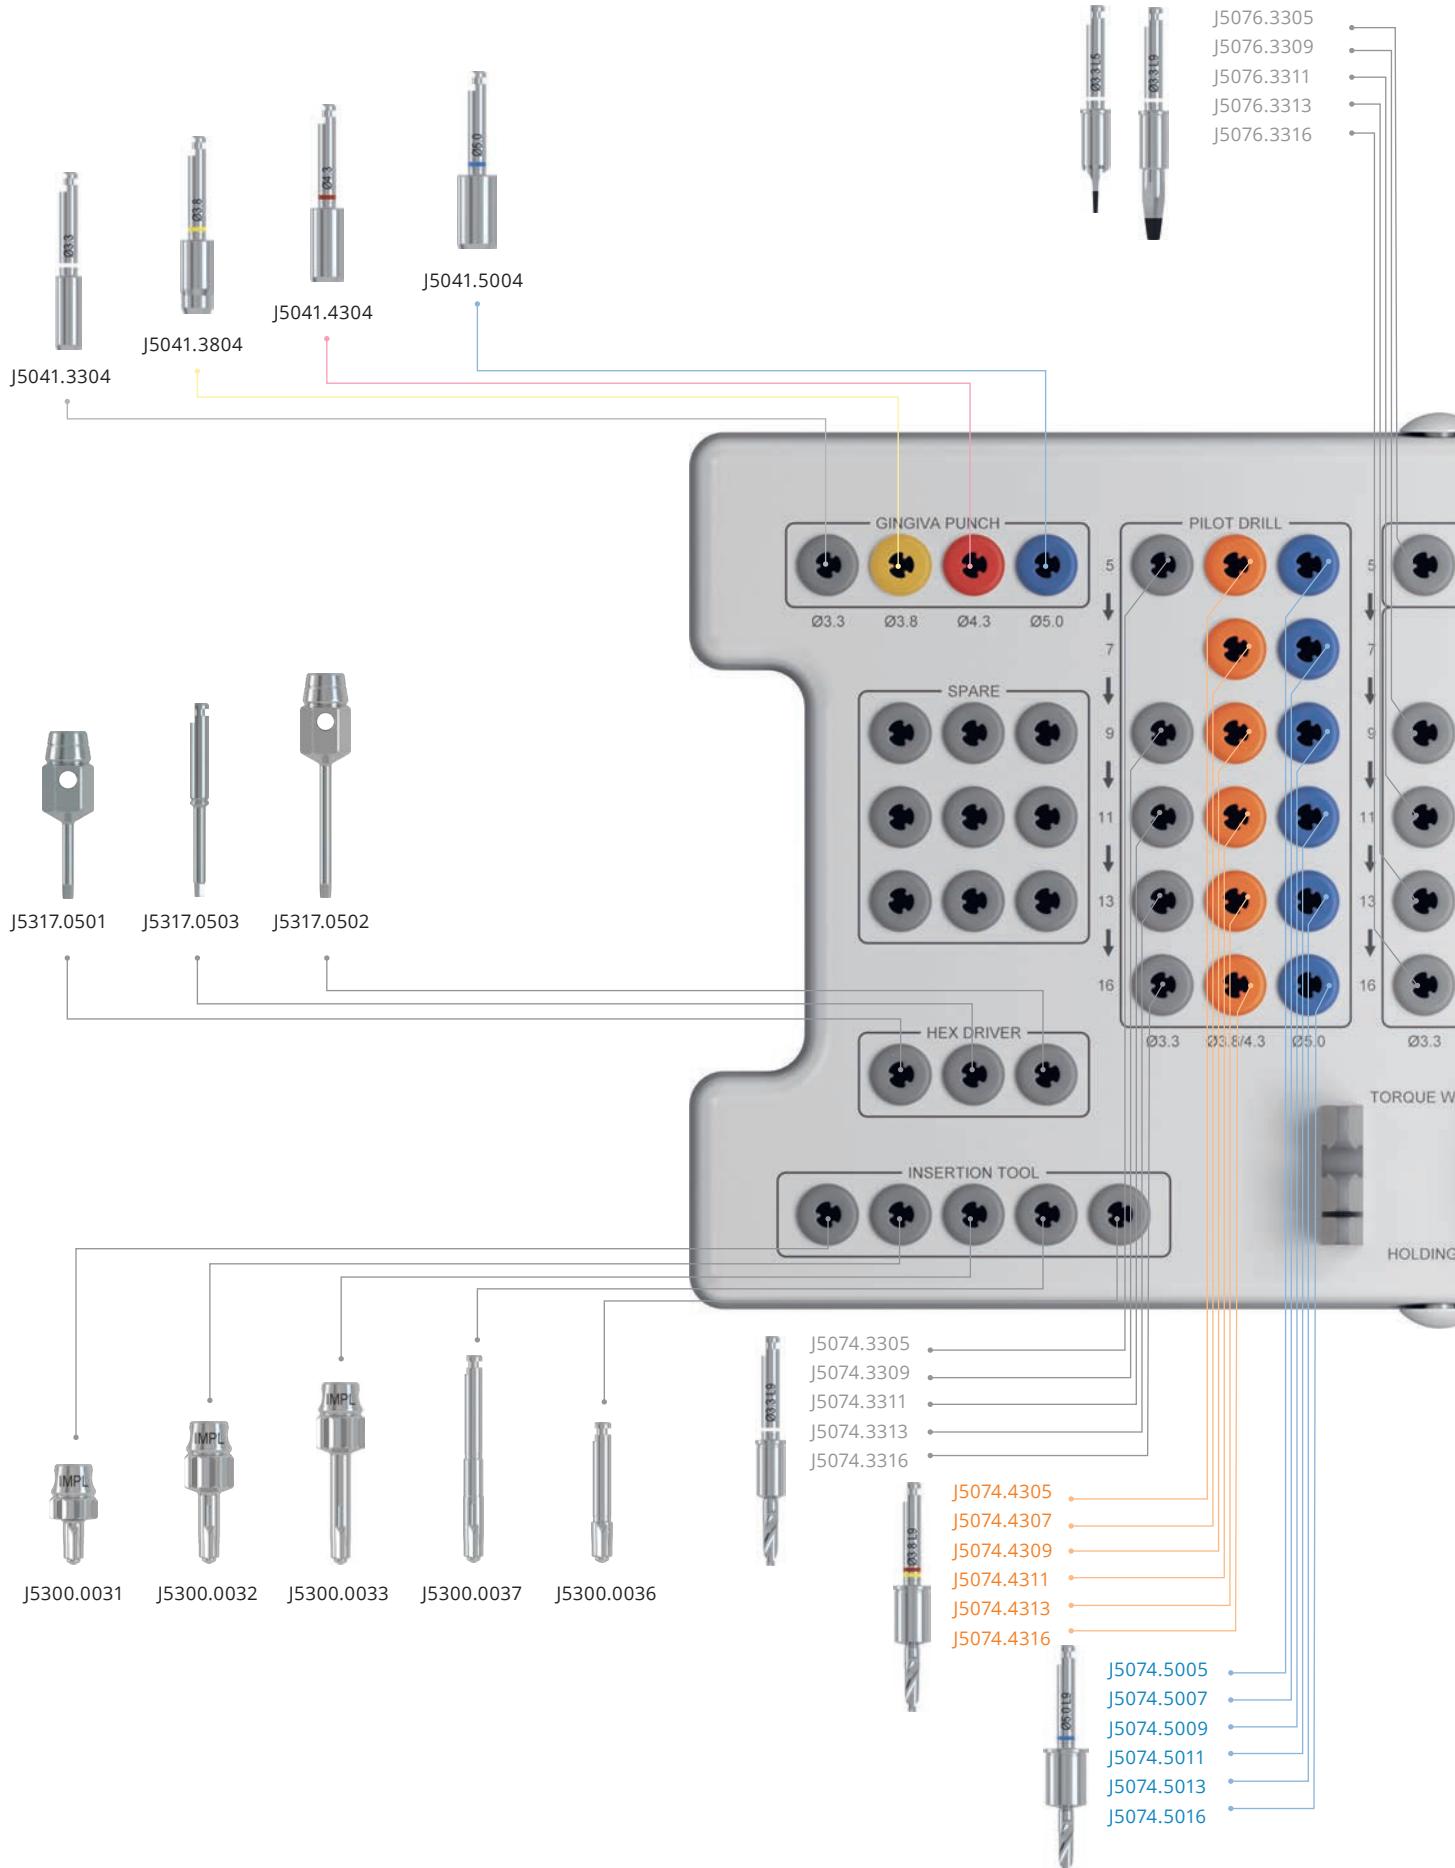
	Article	Art. No.	$\emptyset$	L
	<b>Drill PROGRESSIVE-LINE Flex</b> resterilizable  <b>Material</b> Stainless steel	J5079.3300	3.3 mm	
		J5079.3800	3.8 mm	
		J5079.4300	4.3 mm	
		J5079.5000	5.0 mm	
	<b>Profile drill PROGRESSIVE-LINE Flex</b> resterilizable  <b>Material</b> Stainless steel	J5080.3300	3.3 mm	
		J5080.3800	3.8 mm	
		J5080.4300	4.3 mm	
		J5080.5000	5.0 mm	
	<b>Wrench adapter</b>  <b>Material</b> Stainless steel	J5002.0013	-	11 mm

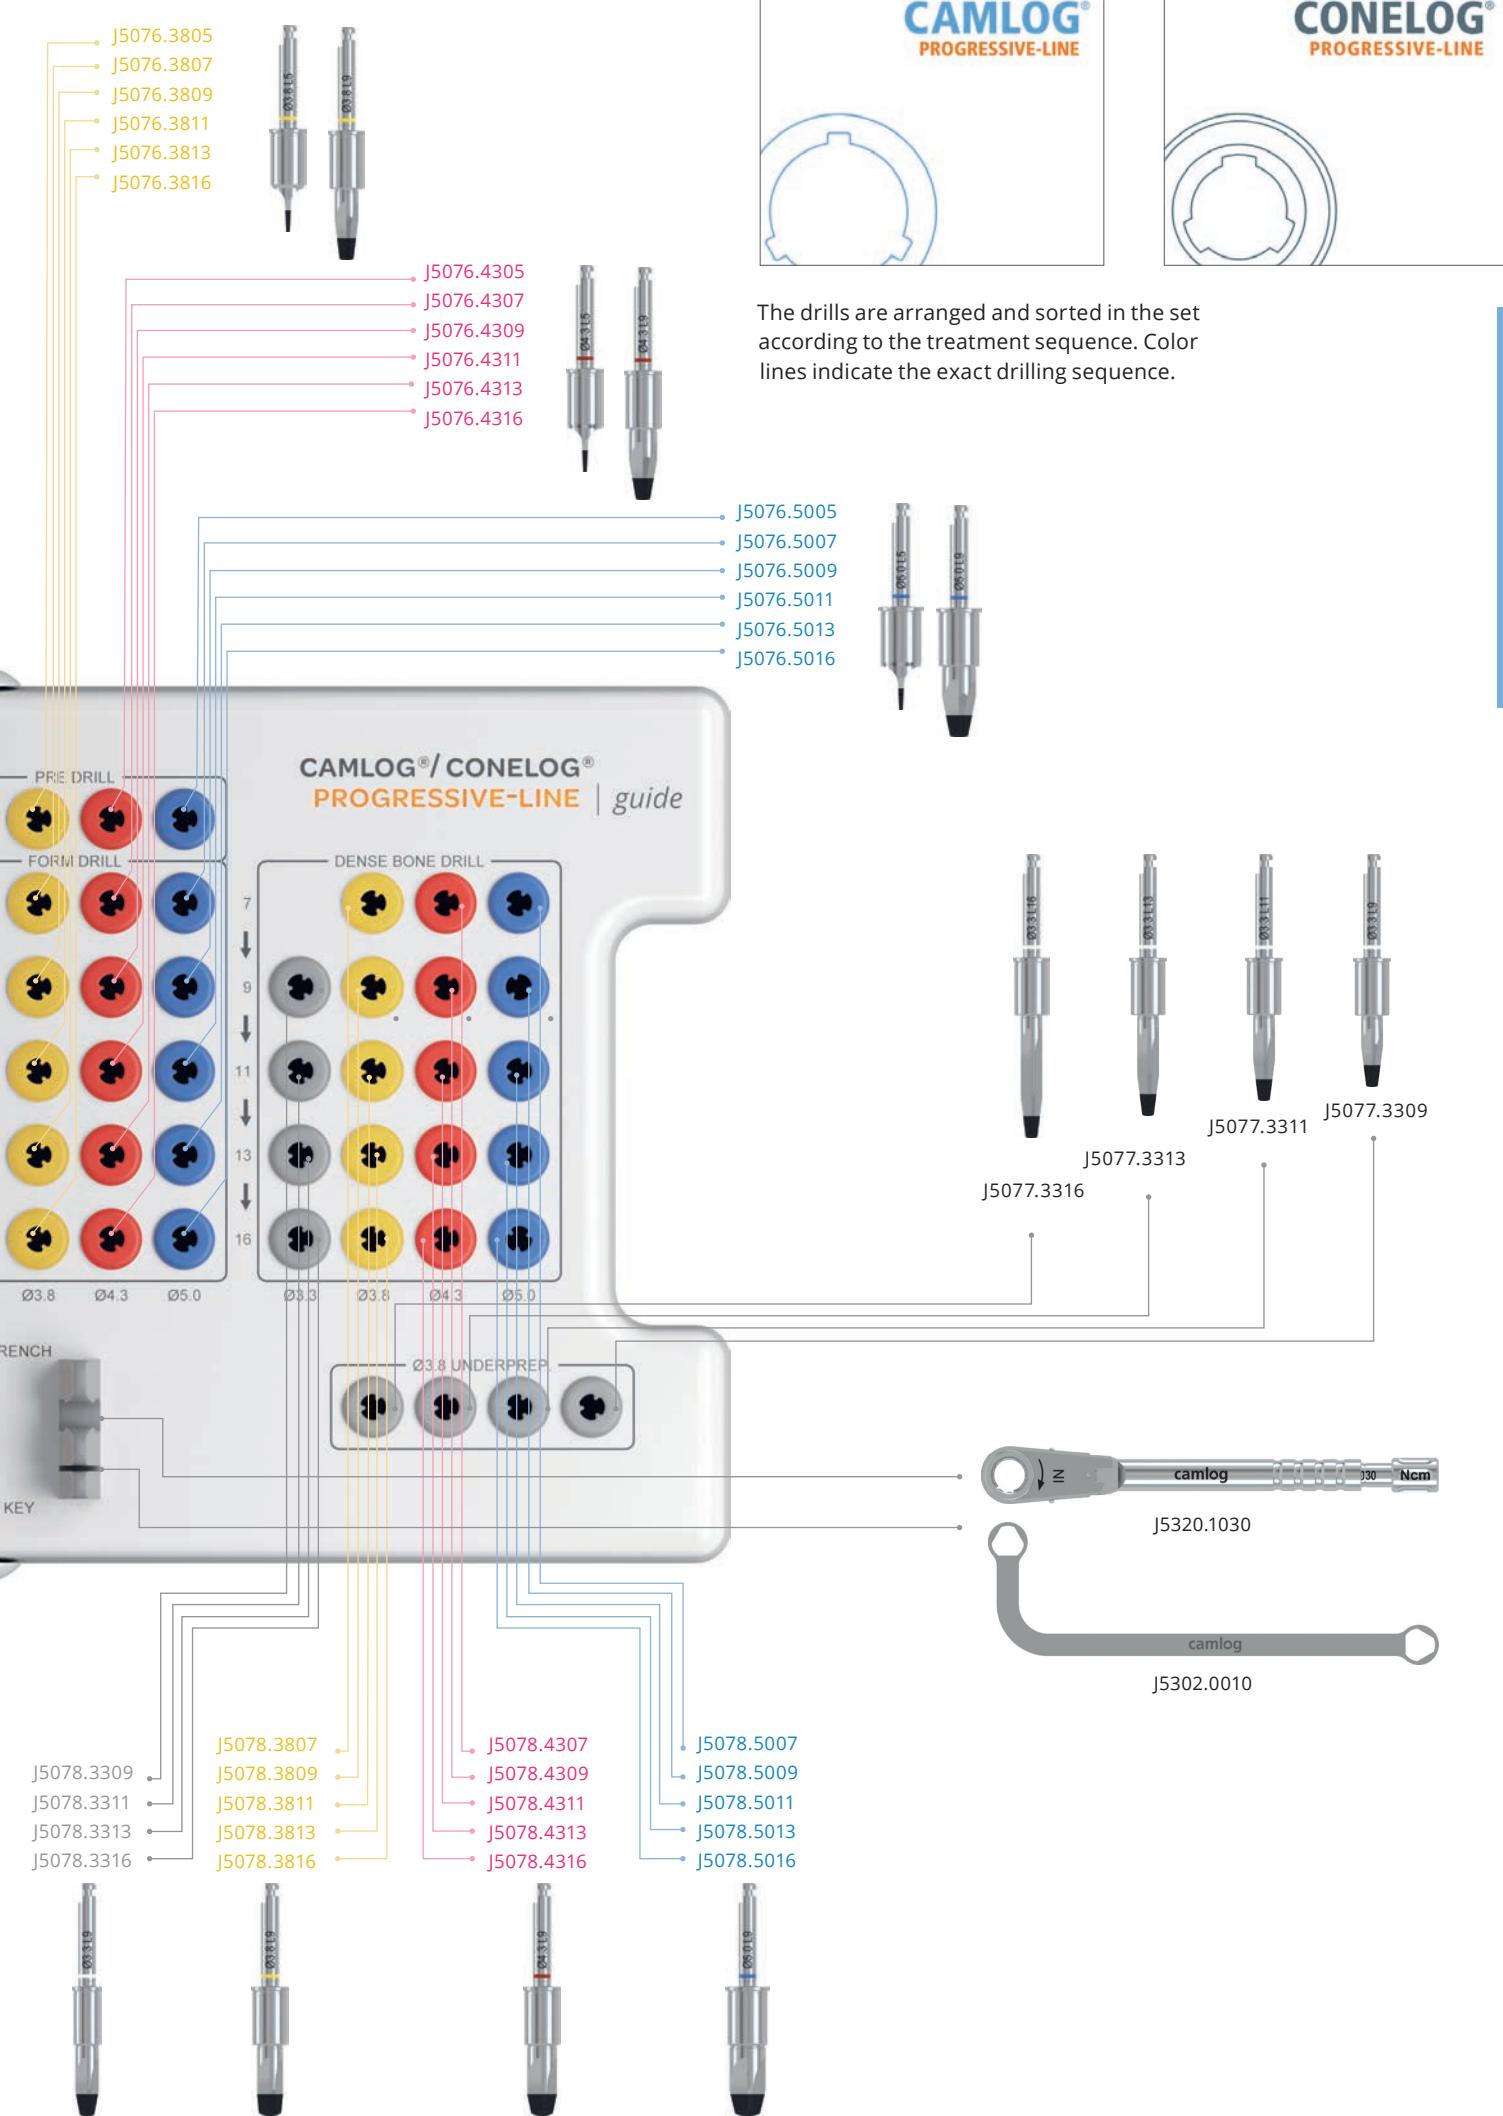
Preparation of the Implant bed with PROGRESSIVE-LINE Flex instruments is also identical for CAMLOG® and CONELOG® PROGRESSIVE-LINE Implants.

# PROGRESSIVE-LINE

Guide System Surgery set CAMLOG®/CONELOG®

**NEW**





# PROGRESSIVE-LINE

## Guide System

	Article	Art. No.
	Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content	J5300.8919

	Article	Art. No.	Ø	L
	Guide System gingiva punch PROGRESSIVE-LINE resterilizable	J5041.3304	3.3 mm	
	Material Stainless steel	J5041.3804	3.8 mm	
		J5041.4304	4.3 mm	-
		J5041.5004*	5.0 mm	
	Guide System pilot drill PROGRESSIVE-LINE resterilizable	J5074.3305	3.3 mm	5 mm
		J5074.3309		9 mm
		J5074.3311		11 mm
		J5074.3313		13 mm
		J5074.3316	3.8 mm	16 mm
		J5074.4305		5 mm
		J5074.4307		7 mm
		J5074.4309		9 mm
		J5074.4311	4.3 mm	11 mm
		J5074.4313		13 mm
		J5074.4316		16 mm
		J5074.5005*		5 mm
		J5074.5007*		7 mm
		J5074.5009*		9 mm
		J5074.5011*		11 mm
		J5074.5013*	5.0 mm	13 mm
		J5074.5016*		16 mm

\* product availability expected for end of Q1/2021

### Notes

CAMLOG® PROGRESSIVE-LINE Implants with Art. No. K1075.xxxx with screw-mounted insertion post can be used with the PROGRESSIVE-LINE Guide System.

	Article	Art. No.	$\varnothing$	L
	Guide System pre-drill PROGRESSIVE-LINE resterilizable	J5076.3305	3.3 mm	5 mm
	Material Stainless steel	J5076.3805	3.8 mm	
		J5076.4305	4.3 mm	
		J5076.5005*	5.0 mm	
	Guide System form drill PROGRESSIVE-LINE resterilizable	J5076.3311	3.3 mm	11 mm
	Material Stainless steel	J5076.3313		13 mm
		J5076.3316		16 mm
		J5076.3809	3.8 mm	9 mm
		J5076.3811		11 mm
		J5076.3813		13 mm
		J5076.3816		16 mm
		J5076.4309	4.3 mm	9 mm
		J5076.4311		11 mm
		J5076.4313		13 mm
		J5076.4316		16 mm
		J5076.5009*	5.0 mm	9 mm
		J5076.5011*		11 mm
		J5076.5013*		13 mm
		J5076.5016*		16 mm
	Guide System dense bone drill PROGRESSIVE-LINE resterilizable	J5078.3311	3.3 mm	11 mm
	Material Stainless steel	J5078.3313		13 mm
		J5078.3316		16 mm
		J5078.3809	3.8 mm	9 mm
		J5078.3811		11 mm
		J5078.3813		13 mm
		J5078.3816		16 mm
		J5078.4309	4.3 mm	9 mm
		J5078.4311		11 mm
		J5078.4313		13 mm
		J5078.4316		16 mm
		J5078.5009*	5.0 mm	9 mm
		J5078.5011*		11 mm
		J5078.5013*		13 mm
		J5078.5016*		16 mm
	Guide System form drill for Ø 3.8 mm under preparation PROGRESSIVE-LINE resterilizable	J5077.3309	3.3 mm	9 mm
	Material Stainless steel	J5077.3311		11 mm
		J5077.3313		13 mm
		J5077.3316		16 mm

\* product availability expected for end of Q1/2021

# PROGRESSIVE-LINE

## Guide System

	Article	Art. No.	$\emptyset$	L
	Guide System template drill PROGRESSIVE-LINE for Guide System guiding sleeve	J3753.3300	3.3 mm	-
	<b>Material</b> Stainless steel	J3753.4300	3.8 mm 4.3 mm	-
		J3753.5000*	5.0 mm	-
	Guide System guiding sleeve PROGRESSIVE-LINE** (2 units)	J3754.3301	3.3 mm	-
	<b>Material</b> Titanium alloy	J3754.3801	3.8 mm	-
		J3754.4301	4.3 mm	-
		J3754.5001*	5.0 mm	-
	Guide System setting tool PROGRESSIVE-LINE for Guide System guiding sleeve	J3717.3300	3.3 mm	-
	<b>Material</b> Stainless steel	J3717.4300	3.8 mm 4.3 mm	-
		J3717.5000*	5.0 mm	-
	Guide System check-up pin PROGRESSIVE-LINE for Guide System guiding sleeve	J5301.3310	3.3 mm	-
	<b>Material</b> Stainless steel	J5301.4310	3.8 mm 4.3 mm	-
		J5301.5010*	5.0 mm	-
	Guide System CAMLOG® Insertion post, screw-mounted for CAMLOG® Lab implant/implant analog, incl. fixing screw (2 units)	K2026.3303	3.3 mm	-
	<b>Material</b> Titanium alloy	K2026.3803	3.8 mm	-
		K2026.4303	4.3 mm	-
		K2026.5003*	5.0 mm	-

\* product availability expected for end of Q1/2021

\*\* only for use with PROGRESSIVE-LINE Implants with screw-mounted insertion post



# SCREW-LINE

## Implants with snap-in insertion post

Article	Art. No.	$\emptyset$	L	A $\emptyset$
 <b>CAMLOG® SCREW-LINE Implant, Promote® incl. snap-in insertion post and cover screw, sterile</b> <b>Material</b> Titanium Grade 4	K1046.3311*	3.3 mm	11 mm	2.7 mm
	K1046.3313*		13 mm	
	K1046.3316*		16 mm	
	K1046.3809*	3.8 mm	9 mm	3.5 mm
	K1046.3811*		11 mm	
	K1046.3813*		13 mm	
	K1046.3816*		16 mm	
	K1046.4309*	4.3 mm	9 mm	3.9 mm
	K1046.4311*		11 mm	
	K1046.4313*		13 mm	
	K1046.4316*		16 mm	
	K1046.5009*	5.0 mm	9 mm	4.6 mm
	K1046.5011*		11 mm	
	K1046.5013*		13 mm	
	K1046.5016*		16 mm	
	K1046.6009*	6.0 mm	9 mm	5.5 mm
	K1046.6011*		11 mm	
	K1046.6013*		13 mm	
	K1046.6016*		16 mm	
 <b>CAMLOG® SCREW-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile</b> <b>Material</b> Titanium Grade 4	K1056.3311**	3.3 mm	11 mm	2.7 mm
	K1056.3313**		13 mm	
	K1056.3316**		16 mm	
	K1056.3809**	3.8 mm	9 mm	3.5 mm
	K1056.3811**		11 mm	
	K1056.3813**		13 mm	
	K1056.3816**		16 mm	
	K1056.4309**	4.3 mm	9 mm	3.9 mm
	K1056.4311**		11 mm	
	K1056.4313**		13 mm	
	K1056.4316**		16 mm	
	K1056.5009**	5.0 mm	9 mm	4.6 mm
	K1056.5011**		11 mm	
	K1056.5013**		13 mm	
	K1056.5016**		16 mm	
	K1056.6009**	6.0 mm	9 mm	5.5 mm
	K1056.6011**		11 mm	
	K1056.6013**		13 mm	
	K1056.6016**		16 mm	

\* Please note: CAMLOG® SCREW-LINE Implants Promote® with Art. No. K1046.xxxx succeed Implants with Art. No. K1044.xxxx. Depending on your country CAMLOG® SCREW-LINE Implants Promote® with Art. No. K1044.xxxx might still be available for a longer period.

\*\* Please note: CAMLOG® SCREW-LINE Implants Promote® plus with Art. No. K1056.xxxx succeed Implants with Art. No. K1054.xxxx. Depending on your country CAMLOG® SCREW-LINE Implants Promote® plus with Art. No. K1054.xxxx might still be available for a longer period.

### Notes

CAMLOG® SCREW-LINE Implants Promote® with Art. No. K1044.xxxx/K1045.xxxx/K1046.xxxx and CAMLOG® SCREW-LINE Implants Promote® plus with Art. No. K1054.xxxx/K1055.xxxx/K1056.xxxx can be used exclusively with the drivers Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034, J5300.0035, J5300.0036 or J5300.0037.

With CAMLOG® SCREW-LINE Implants with the diameters 3.8/4.3/5.0/6.0 mm, the option of Platform Switching is possible.

## Implants with screw-mounted insertion post

Article	Art. No.	$\emptyset$	L	A $\emptyset$
 <b>CAMLOG® SCREW-LINE Implant, Promote®</b> incl. screw-mounted insertion post and cover screw, sterile	K1045.3311	3.3 mm	11 mm	2.7 mm
	K1045.3313		13 mm	
	K1045.3316		16 mm	
	K1045.3809	3.8 mm	9 mm	3.5 mm
	K1045.3811		11 mm	
	K1045.3813		13 mm	
	K1045.3816		16 mm	
	K1045.4309	4.3 mm	9 mm	3.9 mm
	K1045.4311		11 mm	
	K1045.4313		13 mm	
	K1045.4316		16 mm	
	K1045.5009	5.0 mm	9 mm	4.6 mm
	K1045.5011		11 mm	
	K1045.5013		13 mm	
 <b>CAMLOG® SCREW-LINE Implant, Promote® plus</b> incl. screw-mounted insertion post and cover screw, sterile	K1055.3311*	3.3 mm	11 mm	2.7 mm
	K1055.3313*		13 mm	
	K1055.3316*		16 mm	
	K1055.3809*	3.8 mm	9 mm	3.5 mm
	K1055.3811*		11 mm	
	K1055.3813*		13 mm	
	K1055.3816*		16 mm	
	K1055.4309*	4.3 mm	9 mm	3.9 mm
	K1055.4311*		11 mm	
	K1055.4313*		13 mm	
	K1055.4316*		16 mm	
	K1055.5009*	5.0 mm	9 mm	4.6 mm
	K1055.5011*		11 mm	
	K1055.5013*		13 mm	

\* Please note: CAMLOG® SCREW-LINE Implants Promote® plus with Art. No. K1055.xxxx succeed Implants with Art. No. K1053.xxxx. Depending on your country CAMLOG® SCREW-LINE Implants Promote® plus with Art. No. K1053.xxxx might still be available for a longer period.

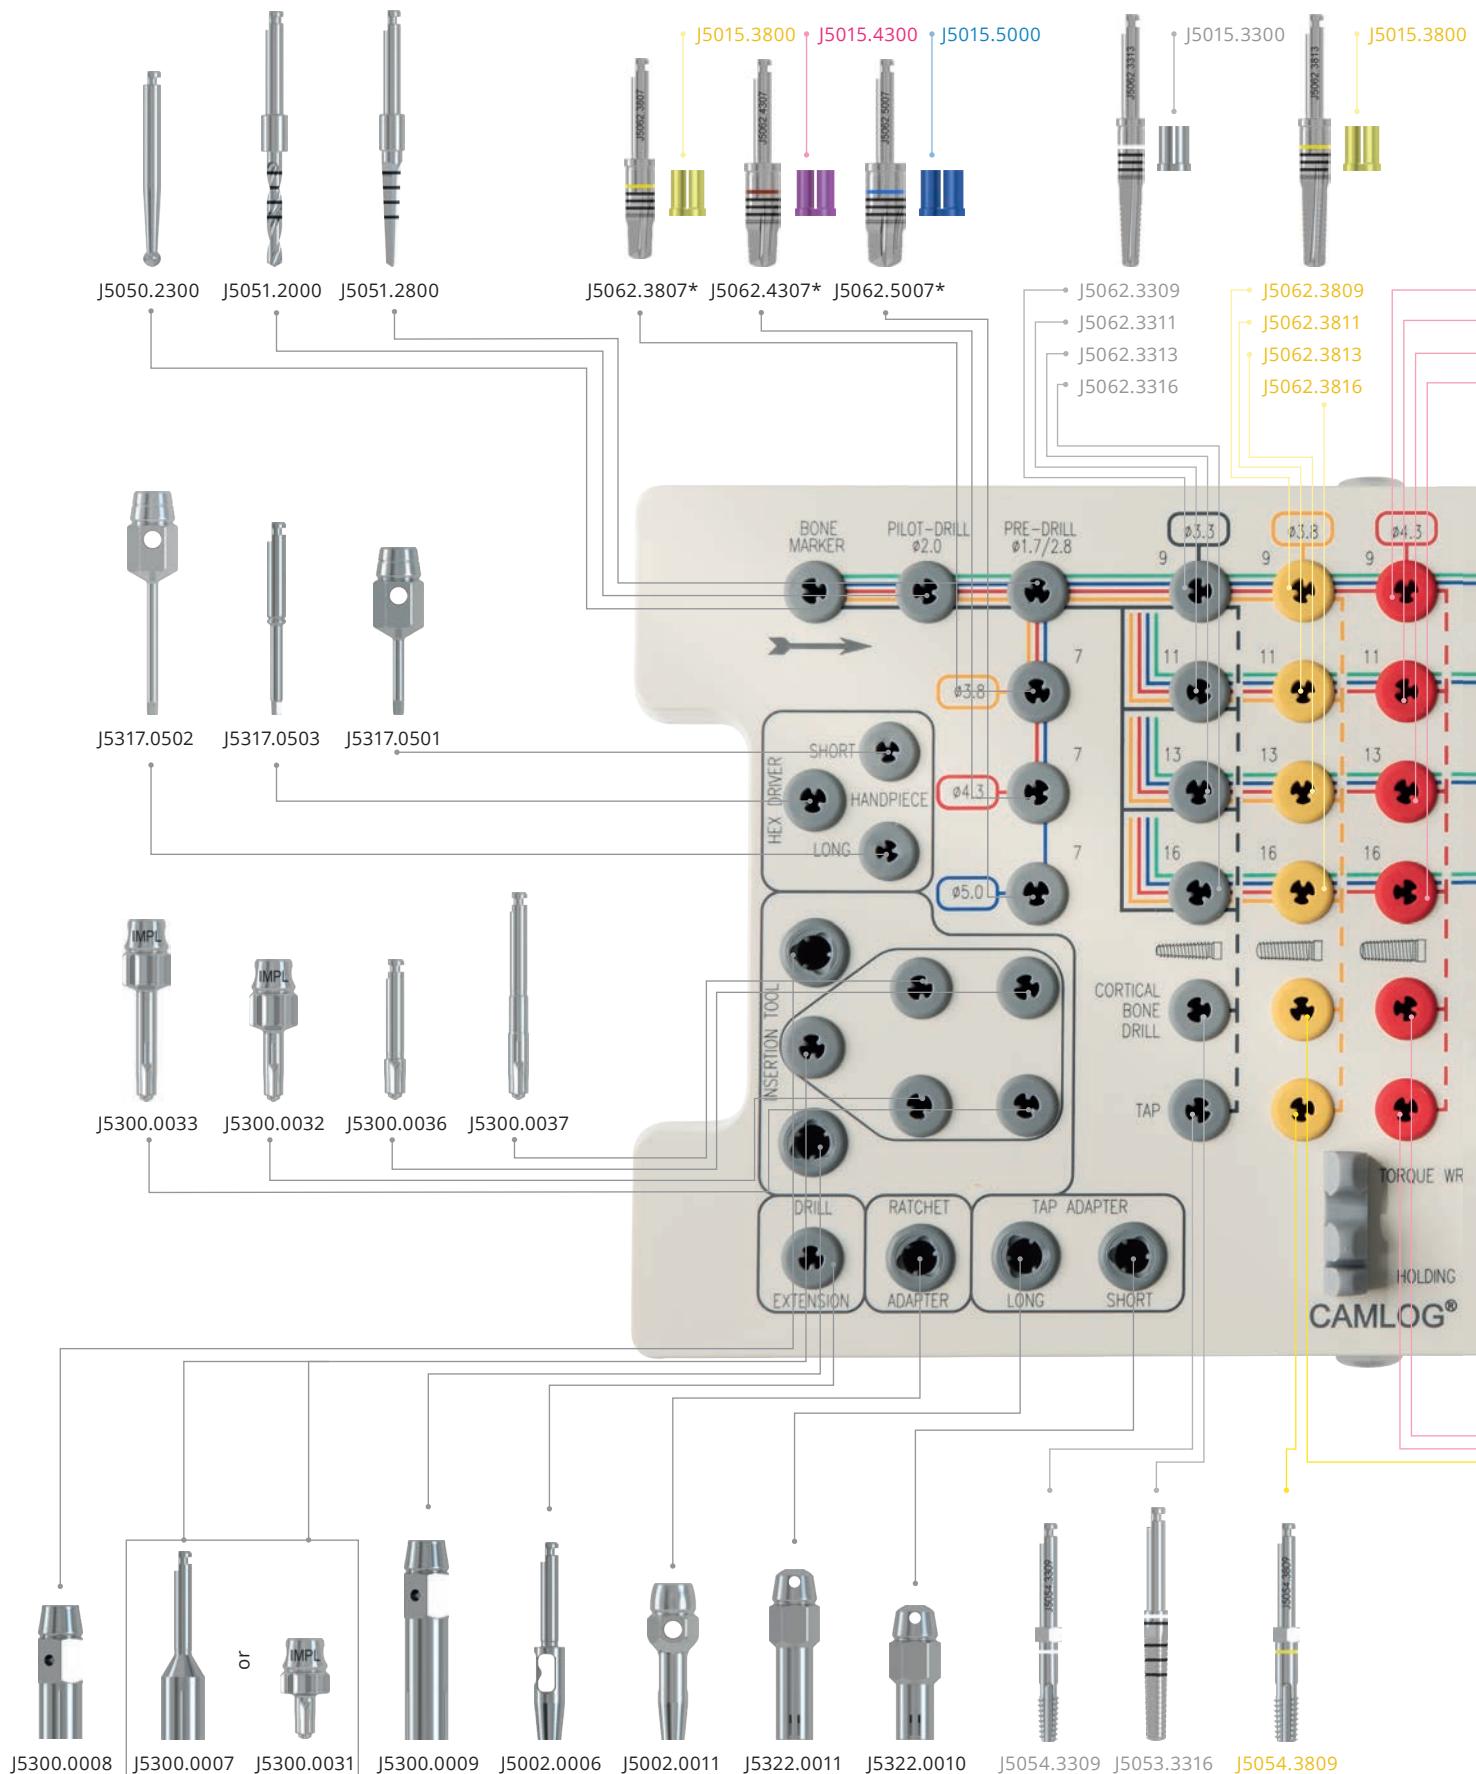
### Notes

CAMLOG® SCREW-LINE Implants Promote® with Art. No. K1044.xxxx/K1045.xxxx/K1046.xxxx and CAMLOG® SCREW-LINE Implants Promote® plus with Art. No. K1054.xxxx/K1055.xxxx/K1056.xxxx can be used exclusively with the drivers Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034, J5300.0035, J5300.0036 or J5300.0037.


With CAMLOG® SCREW-LINE Implants with the diameters 3.8/4.3/5.0/6.0 mm, the option of Platform Switching is possible.

# SCREW-LINE

## Surgery set CAMLOG®/CONELOG®







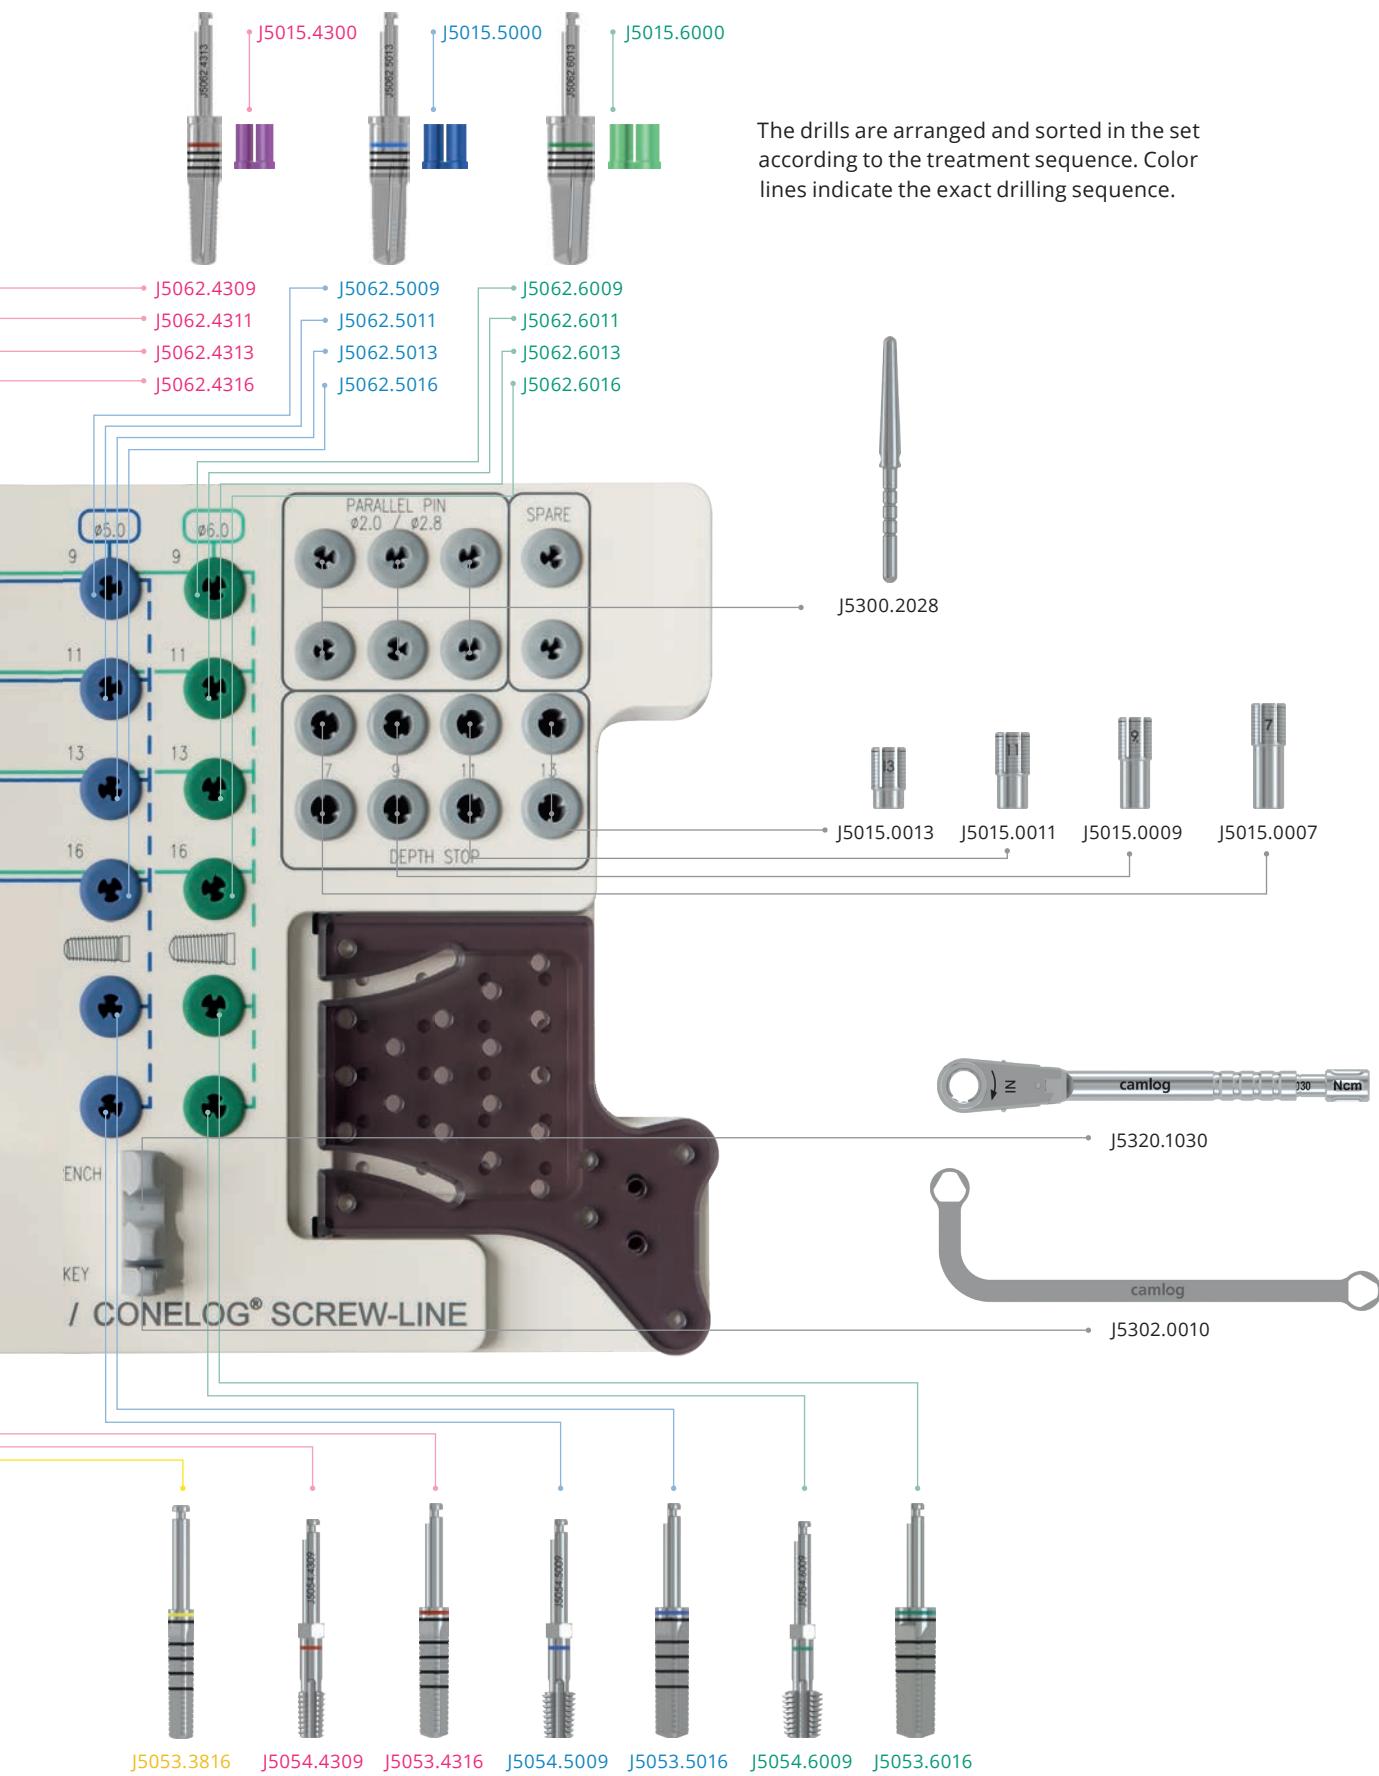\* only for CONELOG® SCREW-LINE Implants length 7 mm



# SCREW-LINE
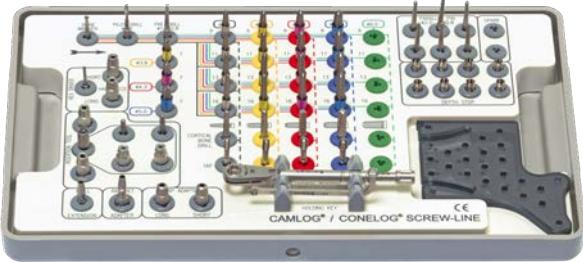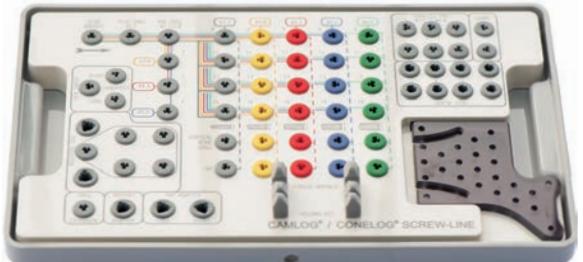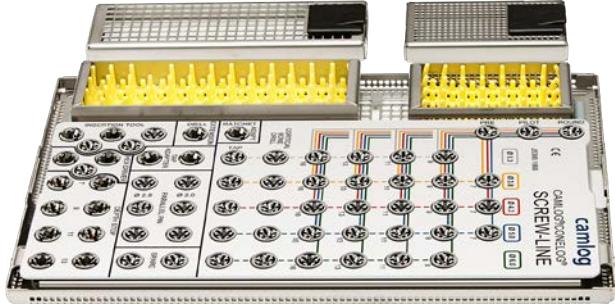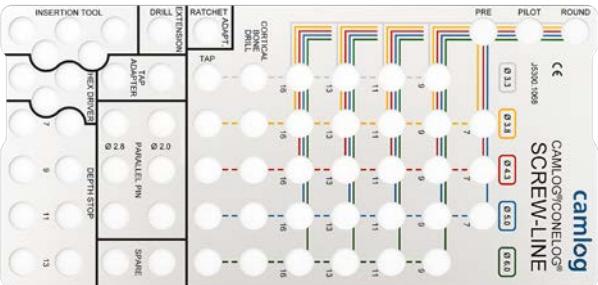
## Surgery set

Article	Art. No.
 <p><b>Surgery set</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b>  contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post (drills and taps for Ø 6.0 mm are not included)</p>	J5300.0063
 <p><b>Surgery tray</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b>  without content</p>	J5300.8916
 <p><b>Surgery wash tray</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b>  incl. pattern, without content</p>	J5300.8968
 <p><b>Pattern for surgery wash tray</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b></p> <p><b>Material</b>  Aluminum</p>	J5300.1068

Preparation of the Implant bed for CAMLOG® SCREW-LINE Implants and for CONELOG® SCREW-LINE Implants is performed with identical instruments.

## Surgical instruments

	Article	Art. No.	$\varnothing$	L
	<b>Form drill SCREW-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5062.3309	3.3 mm	9 mm
		J5062.3311		11 mm
		J5062.3313		13 mm
		J5062.3316		16 mm
		J5062.3809	3.8 mm	9 mm
		J5062.3811		11 mm
		J5062.3813		13 mm
		J5062.3816		16 mm
		J5062.4309	4.3 mm	9 mm
		J5062.4311		11 mm
		J5062.4313		13 mm
		J5062.4316		16 mm
		J5062.5009	5.0 mm	9 mm
		J5062.5011		11 mm
		J5062.5013		13 mm
		J5062.5016		16 mm
		J5062.6009	6.0 mm	9 mm
		J5062.6011		11 mm
		J5062.6013		13 mm
		J5062.6016		16 mm
	<b>Depth stop for form drills</b> PROGRESSIVE-LINE and SCREW-LINE resterilizable  <b>Material</b> Titanium alloy	J5015.3300	3.3 mm	
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
		J5015.6000	6.0 mm	
	<b>Form drill SCREW-LINE</b> Cortical bone resterilizable  <b>Material</b> Stainless steel	J5053.3316	3.3 mm	
		J5053.3816	3.8 mm	
		J5053.4316	4.3 mm	
		J5053.5016	5.0 mm	
		J5053.6016	6.0 mm	
	<b>Tap SCREW-LINE</b> with hexagon, resterilizable  <b>Material</b> Stainless steel	J5054.3309	3.3 mm	
		J5054.3809	3.8 mm	
		J5054.4309	4.3 mm	
		J5054.5009	5.0 mm	
		J5054.6009	6.0 mm	

# SCREW-LINE

## Guide System

Article	Art. No.	$\varnothing$	L
Guide System pilot drill set internal irrigation, sterile (for pilot drilling $\varnothing$ 2.0 mm)	J5063.3311	3.3 mm	11 mm (incl. 5 and 9 mm)**
	J5063.3313		13 mm (incl. 5, 9 and 11 mm)**
	J5064.3316*		16 mm
	J5063.4309	3.8 mm	9 mm (incl. 5 mm)**
		4.3 mm	
	J5063.4311	3.8 mm	11 mm (incl. 5 and 9 mm)**
		4.3 mm	
	J5063.4313	3.8 mm	13 mm (incl. 5, 9 and 11 mm)**
		4.3 mm	
	J5064.4316*	3.8 mm	16 mm
		4.3 mm	

\* Necessary Guide System pilot drill for Implant length 16 mm, following obligatory prior use of the pilot drill set length 13 mm.

\*\* All Guide System pilot drill sets include a 5 mm long pilot drill, as well as all pilot drills necessary for the selected Implant length.

Article	Art. No.	$\varnothing$	L
Guide System surgery set, SCREW-LINE internal irrigation, sterile	J5065.3311	3.3 mm	11 mm (incl. 5 and 9 mm)****
	J5065.3313		13 mm (incl. 5, 9 and 11 mm)****
	J5066.3316***		16 mm
	J5065.3809	3.8 mm	9 mm (incl. 5 mm)****
	J5065.3811		11 mm (incl. 5 and 9 mm)****
	J5065.3813	4.3 mm	13 mm (incl. 5, 9 und 11 mm)****
	J5066.3816***		16 mm
	J5065.4309	4.3 mm	9 mm (incl. 5 mm)****
	J5065.4311		11 mm (incl. 5 and 9 mm)****
	J5065.4313		13 mm (incl. 5, 9 and 11 mm)****
	J5066.4316***		16 mm

\*\*\* Necessary Guide System form drill for Implant length 16 mm, following obligatory prior use of the Guide System surgery set length 13 mm.

\*\*\*\* All Guide System surgery sets include a 5 mm long pre-drill, as well as all form drills necessary for the selected Implant length.

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

### Notes

CAMLOG® SCREW-LINE Implants with Art. No. K1045.xxxx/K1055.xxxx with screw-mounted insertion post can be used with the SCREW-LINE Guide System.

The SCREW-LINE Guide System can only be used for Implant diameters 3.3/3.8/4.3 mm.

	Article	Art. No.	$\emptyset$	L
	<b>Guide System form drill, SCREW-LINE, Cortical Bone internal irrigation, sterile</b>  <b>Material</b> Stainless steel	J5068.3311	3.3 mm	11 mm
		J5068.3313		13 mm
		J5068.3316		16 mm
		J5068.3809	3.8 mm	9 mm
		J5068.3811		11 mm
		J5068.3813		13 mm
		J5068.3816		16 mm
		J5068.4309	4.3 mm	9 mm
		J5068.4311		11 mm
		J5068.4313		13 mm
		J5068.4316		16 mm
	<b>Guide System gingiva punch sterile</b>  <b>Material</b> Stainless steel	J5041.3303	3.3 mm	-
		J5041.3803	3.8 mm	
		J5041.4303	4.3 mm	
	<b>Guide System guiding sleeve height 3.0 mm (2 units)</b>  <b>Material</b> Titanium alloy	J3734.3303*	3.3 mm	-
		J3734.3803*	3.8 mm	
		J3734.4303*	4.3 mm	

\* only for use with SCREW-LINE Implants with screw-mounted insertion post

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

# SCREW-LINE

## Guide System

	Article	Art. No.	$\varnothing$	L
	<b>Guide System CAMLOG® Insertion post, screw-mounted</b> for CAMLOG® Lab implant/implant analog, incl. fixing screw (2 units)	K2026.3303	3.3 mm	
	<b>Material</b> Titanium alloy	K2026.3803	3.8 mm	-
	<b>Material</b> Titanium alloy	K2026.4303	4.3 mm	
	<b>Guide System template drill</b> for Guide System Guiding sleeve	J3733.3300	3.3 mm	
	<b>Material</b> Stainless steel	J3733.4300	3.8 mm	-
	<b>Material</b> Stainless steel	J3733.4300	4.3 mm	
	<b>Guide System seating tool</b> for Guide System Guiding sleeve	J3716.3300	3.3 mm	
	<b>Material</b> Stainless steel	J3716.4300	3.8 mm	-
	<b>Material</b> Stainless steel	J3716.4300	4.3 mm	
	<b>Guide System check-up pin</b> for Guide System Guiding sleeve	J5301.3300	3.3 mm	
	<b>Material</b> Stainless steel	J5301.4300	3.8 mm	-
	<b>Material</b> Stainless steel	J5301.4300	4.3 mm	
	<b>Drill extension</b> ISO shaft, for instruments with internal irrigation	J5002.0005	-	26.6 mm
	<b>Material</b> Stainless steel			

# General surgical instruments

	Article	Art. No.	$\emptyset$	L
	<b>Round bur</b> resterilizable <b>Material</b> Stainless steel	J5050.2300	2.3 mm	-
	<b>Point drill</b> resterilizable <b>Material</b> Stainless steel	B1012*	1.5 mm	30.0 mm
	<b>Pilot drill</b> without coil, resterilizable <b>Material</b> Stainless steel	J5051.2003	2.0 mm	-
	<b>Pilot drill SCREW-LINE</b> resterilizable <b>Material</b> Stainless steel	J5051.2000	2.0 mm	-
	<b>Pre-drill SCREW-LINE</b> resterilizable <b>Material</b> Stainless steel	J5051.2800	1.7 – 2.8 mm	-

\* Manufacturer: AXIS biidental SA, Les Rosées 5, 2336 Les Bois, Switzerland

# General surgical instruments

	Article	Art. No.	$\emptyset$	L
	Depth stop SCREW-LINE for pilot drill (J5051.2000) and pre-drill (J5051.2800), resterilizable	J5015.0009	-	9 mm
	Material Stainless steel	J5015.0011		11 mm
		J5015.0013		13 mm
	Bone profiler Material Stainless steel	$\emptyset$ 5.0 mm	J5003.3350	3.3 mm
		$\emptyset$ 6.0 mm	J5003.4360	3.8 mm 4.3 mm
		$\emptyset$ 7.0 mm	J5003.5070	5.0 mm
	CAMLOG® Guiding pin for bone profiler Material Titanium alloy	J5002.3300 J5002.3800 J5002.4300 J5002.5000	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Countersink Material Stainless steel	$\emptyset$ 4.6 mm	J5006.3346	3.3 mm
		$\emptyset$ 5.2 mm	J5006.3852	3.8 mm
		$\emptyset$ 5.6 mm	J5006.4356	4.3 mm
		$\emptyset$ 6.3 mm	J5006.5063	5.0 mm
	Baring drill for cover screw Material Stainless steel	J5004.3300	3.3 mm	-
		J5004.3800	3.8 mm	-
		J5004.4300	4.3 mm	-
		J5004.5000	5.0 mm	-

	Article	Art. No.	Dimension
	<b>Paralleling pin SCREW-LINE</b> with depth marks <b>Material</b> Titanium alloy	J5300.2028	$\varnothing$ 1.7 – 2.8 mm/ 2.0 mm
	<b>Drill extension</b> ISO shaft (not for drills with internal irrigation) <b>Material</b> Stainless steel	J5002.0006	26.5 mm
	<b>Tap adapter, short</b> for tap SCREW-LINE <b>Material</b> Stainless steel	J5322.0010	18.0 mm
	<b>Tap adapter, long</b> for tap SCREW-LINE <b>Material</b> Stainless steel	J5322.0011	23.0 mm

## General surgical instruments

	Article	Art. No.	Dimension
	<b>Driver, extra short</b> for screw Implants, manual/wrench <b>Material</b> Stainless steel	J5300.0031*	13.7 mm
	<b>Driver, short</b> for screw Implants, manual/wrench <b>Material</b> Stainless steel	J5300.0032*	19.2 mm
	<b>Driver, long</b> for screw Implants, manual/wrench <b>Material</b> Stainless steel	J5300.0033*	24.8 mm
	<b>Driver, short</b> for screw Implants, with ISO shaft for angled hand piece (without hexagon at the shaft) <b>Material</b> Stainless steel	J5300.0036*	19.1 mm
	<b>Driver, long</b> for screw Implants, with ISO shaft for angled hand piece (without hexagon at the shaft) <b>Material</b> Stainless steel	J5300.0037*	28.2 mm
	<b>Driver, short</b> for screw Implants, with ISO-shaft for angled hand piece, for Hexagon clamping system <b>Material</b> Stainless steel	J5300.0034*	19.1 mm
	<b>Driver, long</b> for screw Implants, with ISO-shaft for angled hand piece, for Hexagon clamping system <b>Material</b> Stainless steel	J5300.0035*	28.2 mm

\* only for use with CAMLOG® PROGRESSIVE-LINE Implants with Art. No. K1075.xxxx, K1076.xxxx and CAMLOG® SCREW-LINE Implants with Art. No. K1044.xxxx, K1045.xxxx, K1046.xxxx, K1054.xxxx, K1055.xxxx and K1056.xxxx.

	Article	Art. No.	Dimension
	<b>Cardanic driver (30°)</b> adjustable length  <b>Material</b> Stainless steel	J5300.0038*	-
	<b>PickUp instrument</b> holder for carrying Implants  <b>Material</b> Stainless steel	J5300.0030**	-
	<b>Adapter</b> ISO shaft for angled hand piece  <b>Material</b> Stainless steel	J5002.0011	21.0 mm

\* only for use with CAMLOG® PROGRESSIVE-LINE Implants with Art. No. K1075.xxxx, K1076.xxxx and CAMLOG® SCREW-LINE Implants with Art. No. K1044.xxxx, K1045.xxxx, K1046.xxxx, K1054.xxxx, K1055.xxxx and K1056.xxxx.

\*\* only for use with CAMLOG® PROGRESSIVE-LINE Implants (with snap-in insertion post) with Art. No. K1076.xxxx and CAMLOG® SCREW-LINE Implants with Art. No. K1042.xxxx, K1046.xxxx, K1052.xxxx and K1056.xxxx.

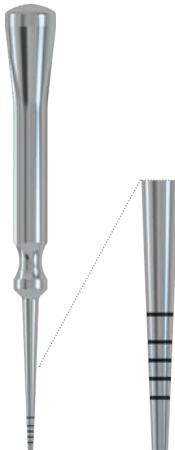
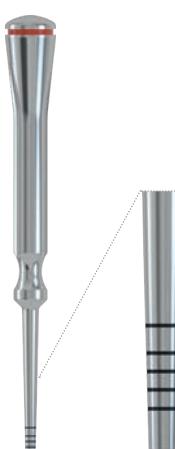
# General surgical instruments

	Article	Art. No.	$\varnothing$	Dimension
	<b>Holding key for insertion post</b> <b>Material</b> Stainless steel	J5302.0010	-	-
	<b>CAMLOG® Adapter for screw Implants, short for CAMLOG® Implants</b> <b>Material</b> Stainless steel	K5302.3311 K5302.3811 K5302.4311 K5302.6011	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm	29.8 mm
	<b>CAMLOG® Adapter for screw Implants, long for CAMLOG® Implants</b> <b>Material</b> Stainless steel	K5302.3310 K5302.3810 K5302.4310	3.3 mm 3.8 mm 4.3 mm	34.8 mm
	<b>Holding sleeve for screw Implants color-coded</b> <b>Material</b> Titanium alloy	J5302.3300 J5302.3800 J5302.4300 J5302.5000 J5302.6000	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm	-
	<b>Screwdriver hex, extra short, manual/wrench</b> <b>Material</b> Stainless steel	J5317.0510	-	14.5 mm
	<b>Screwdriver hex, short, manual/wrench</b> <b>Material</b> Stainless steel	J5317.0501	-	22.5 mm
	<b>Screwdriver hex, long, manual/wrench</b> <b>Material</b> Stainless steel	J5317.0502	-	30.3 mm

	Article	Art. No.	Dimension
	<b>Screwdriver</b> hex, short, ISO shaft  <b>Material</b> Stainless steel	J5317.0504	18.0 mm
	<b>Screwdriver</b> hex, long, ISO shaft  <b>Material</b> Stainless steel	J5317.0503	26.0 mm
	<b>Manual screwdriver, hex</b> without wrench head connection  <b>Material</b> Stainless steel	J5317.0511	23.0 mm
	<b>Cleaning needle</b> for instruments with internal irrigation  <b>Material</b> Stainless steel	J5002.0012	-
	<b>Cleaning cannula</b> for drills with internal irrigation  <b>Material</b> Stainless steel	J5002.0020	-

# SCREW-LINE

## Osteotomy set

	Article	Art. No.	$\emptyset$
	<b>Osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight convex</b> <b>Material</b> Stainless steel	J5418.0020	-
	<b>Pre-Osteotome SCREW-LINE straight convex</b> <b>Material</b> Stainless steel	J5417.2800*	1.7 – 2.8 mm
	<b>Osteotome SCREW-LINE straight convex</b> <b>Material</b> Stainless steel	J5418.3300* J5418.3800* J5418.4300* J5418.5000* J5418.6000*	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm

\* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight convex.

	Article	Art. No.	$\varnothing$
	<b>Osteotomy set</b> <b>CAMLOG®/CONELOG® SCREW-LINE</b> angled convex  <b>Material</b> Stainless steel	J5418.0030	-
	<b>Pre-Osteotome SCREW-LINE</b> straight convex  <b>Material</b> Stainless steel	J5417.2800*	1.7 – 2.8 mm
	<b>Osteotome SCREW-LINE</b> angled convex  <b>Material</b> Stainless steel	J5418.3310* J5418.3810* J5418.4310* J5418.5010* J5418.6010*	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm



\* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex.

# SCREW-LINE
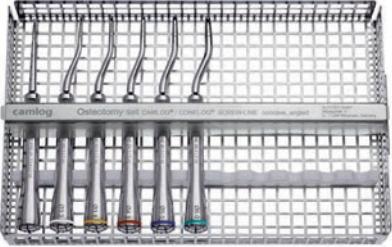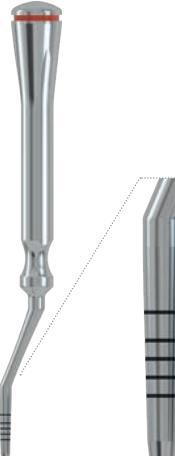
## Osteotomy set


	Article	Art. No.	$\emptyset$
	<b>Osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave</b> <b>Material</b> Stainless steel	J5420.0020	-
	<b>Pre-Osteotome SCREW-LINE straight concave</b> <b>Material</b> Stainless steel	J5419.2800*	1.7 – 2.8 mm
	<b>Osteotome SCREW-LINE straight concave</b> <b>Material</b> Stainless steel	J5420.3300* J5420.3800* J5420.4300* J5420.5000* J5420.6000*	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm

\* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave.

	Article	Art. No.	$\emptyset$
	<b>Osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave</b> <b>Material</b> Stainless steel	J5420.0030	-
	<b>Pre-Osteotome SCREW-LINE straight concave</b> <b>Material</b> Stainless steel	J5419.2800*	1.7 – 2.8 mm
	<b>Osteotome SCREW-LINE angled concave</b> <b>Material</b> Stainless steel	J5420.3310* J5420.3810* J5420.4310* J5420.5010* J5420.6010*	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm

\* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave.

## ALTApin set

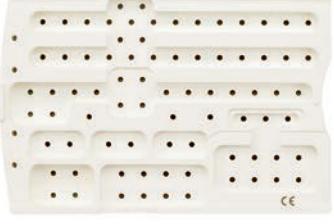	Article	Art. No.
	<b>ALTApin set</b> Membrane fixation system, resterilizable <b>Material</b> Plastic/Titanium alloy/Stainless steel	M5600.0110
	<b>ALTApin Tray</b> (without content) <b>Material</b> Plastic	M5600.0210
	<b>ALTApin applicator, straight</b> incl. activator <b>Material</b> Stainless steel	M5100.0010*
	<b>ALTApin applicator, angled 90°</b> incl. activator <b>Material</b> Stainless steel	M5100.0030
	<b>ALTApin applicator, straight,</b> <b>work element</b> incl. activator <b>Material</b> Stainless steel	M5200.0010

\* These products are included in the ALTApin set.

	Article	Art. No.
	<b>ALTApin pricker</b> <b>Material</b> Stainless steel	M5100.0050*
	<b>ALTApin membrane fixator</b> <b>Material</b> Stainless steel	M5100.0070*
	<b>ALTApin surgery mallet</b> <b>Material</b> Stainless steel/POM	M5100.0100
	<b>ALTApin single patient drill, ISO shaft</b> <b>Material</b> Stainless steel	M5500.0050

\* These products are included in the ALTApin set.

## ALTApin set

	Article	Art. No.
	<b>ALTApin pricker, insert</b>  <b>Material</b> Stainless steel	M5200.0055*
	<b>ALTApin magazine</b> 7 titanium pins, sterile, 1 unit  <b>Material</b> Titanium alloy	M1000.0050*
	<b>ALTApin magazine</b> 7 titanium pins, sterile, 3 units  <b>Material</b> Titanium alloy	M1000.0100

\* These products are included in the ALTApin set.

## Cover screws

	Article	Art. No.	$\emptyset$
	<b>CAMLOG® Implant cover screw</b>  Material Titanium alloy	J2019.3300 J2019.3800 J2019.4300 J2019.5000 J2019.6000	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm

## Healing caps

	Article	Art. No.	$\emptyset$	GH	G $\emptyset$
	<b>CAMLOG® Healing cap, cylindrical sterile</b>  Material Titanium alloy	J2015.3320 J2015.3340 J2015.3820 J2015.3840 J2015.3860* J2015.4320 J2015.4340 J2015.4360* J2015.5020 J2015.5040 J2015.5060* J2015.6020 J2015.6040 J2015.6060*	3.3 mm	2.0 mm 4.0 mm 2.0 mm 4.0 mm 6.0 mm 2.0 mm 4.0 mm 6.0 mm 2.0 mm 4.0 mm 5.0 mm 2.0 mm 4.0 mm 6.0 mm	3.3 mm 3.3 mm 3.8 mm 3.8 mm 3.8 mm 4.3 mm 4.3 mm 4.3 mm 5.0 mm 5.0 mm 5.0 mm 6.0 mm 6.0 mm 6.0 mm
	<b>CAMLOG® Healing cap, wide body sterile</b>  Material Titanium alloy	J2014.3320 J2014.3340 J2014.3820 J2014.3840 J2014.3860 J2014.4320 J2014.4340 J2014.4360 J2014.5020 J2014.5040 J2014.5060 J2014.6020 J2014.6040 J2014.6060	3.3 mm	2.0 mm 4.0 mm 2.0 mm 4.0 mm 6.0 mm 2.0 mm 4.0 mm 6.0 mm 2.0 mm 4.0 mm 5.0 mm 2.0 mm 4.0 mm 6.0 mm	4.5 mm 4.5 mm 4.9 mm 5.0 mm 5.0 mm 5.4 mm 5.5 mm 5.5 mm 6.1 mm 6.2 mm 6.2 mm 7.1 mm 7.2 mm 7.2 mm
	<b>CAMLOG® Healing cap, bottleneck sterile</b>  Material Titanium alloy	J2011.3340 J2011.3840 J2011.3860 J2011.4340 J2011.4360 J2011.5040 J2011.5060 J2011.6040 J2011.6060	3.3 mm	4.0 mm 4.0 mm 6.0 mm 4.0 mm 6.0 mm 4.0 mm 6.0 mm 4.0 mm 6.0 mm	3.5 mm 4.0 mm 4.0 mm 4.5 mm 4.5 mm 5.2 mm 5.2 mm 6.2 mm 6.2 mm

\* suitable for bite registration

# Healing caps

## Platform Switching

	Article	Art. No.	$\emptyset$	GH	G $\emptyset$
 <b>PS</b>	<b>CAMLOG® Healing cap PS, cylindrical</b> sterile, for Platform Switching with CAMLOG® Implants with K article number  <b>Material</b> Titanium alloy	K2005.3820		2.0 mm	3.3 mm
		K2005.3840	3.8 mm	4.0 mm	3.3 mm
		K2005.3860*		6.0 mm	3.3 mm
		K2005.4320		2.0 mm	3.8 mm
		K2005.4340	4.3 mm	4.0 mm	3.8 mm
		K2005.4360*		6.0 mm	3.8 mm
		K2005.5020		2.0 mm	4.4 mm
		K2005.5040	5.0 mm	4.0 mm	4.4 mm
		K2005.5060*		6.0 mm	4.4 mm
		K2005.6020		2.0 mm	5.1 mm
		K2005.6040	6.0 mm	4.0 mm	5.1 mm
		K2005.6060*		6.0 mm	5.1 mm
 <b>PS</b>	<b>CAMLOG® Healing cap PS, wide body</b> sterile, for Platform Switching with CAMLOG® Implants with K article number  <b>Material</b> Titanium alloy	K2004.3840	3.8 mm	4.0 mm	5.0 mm
		K2004.3860		6.0 mm	5.0 mm
		K2004.4340	4.3 mm	4.0 mm	5.5 mm
		K2004.4360		6.0 mm	5.5 mm
		K2004.5040	5.0 mm	4.0 mm	6.2 mm
		K2004.5060		6.0 mm	6.2 mm
		K2004.6040	6.0 mm	4.0 mm	7.2 mm
		K2004.6060		6.0 mm	7.2 mm
 <b>PS</b>	<b>CAMLOG® Healing cap PS, bottleneck</b> sterile, for Platform Switching with CAMLOG® Implants with K article number  <b>Material</b> Titanium alloy	K2001.3840	3.8 mm	4.0 mm	4.0 mm
		K2001.3860		6.0 mm	4.0 mm
		K2001.4340	4.3 mm	4.0 mm	4.5 mm
		K2001.4360		6.0 mm	4.5 mm
		K2001.5040	5.0 mm	4.0 mm	5.2 mm
		K2001.5060		6.0 mm	5.2 mm

\* suitable for bite registration



# Impression taking

	Article	Art. No.	$\varnothing$
	<b>CAMLOG® Impression posts, open tray</b> incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex)  <b>Material</b> Titanium alloy	K2121.3300	3.3 mm
		K2121.3800	3.8 mm
		K2121.4300	4.3 mm
		K2121.5000	5.0 mm
		K2121.6000	6.0 mm
	<b>CAMLOG® Impression posts, closed tray</b> incl. impression cap, bite registration cap and fixing screw  <b>Material</b> Titanium alloy/POM	K2110.3300	3.3 mm
		K2110.3800	3.8 mm
		K2110.4300	4.3 mm
		K2110.5000	5.0 mm
		K2110.6000	6.0 mm
	<b>CAMLOG® Impression posts PS, open tray, for Platform Switching</b> incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex)  <b>Material</b> Titanium alloy	K2119.3800	3.8 mm
		K2119.4300	4.3 mm
		K2119.5000	5.0 mm
		K2119.6000	6.0 mm
	<b>CAMLOG® Impression posts PS, closed tray, for Platform Switching</b> incl. impression cap, bite registration cap and fixing screw  <b>Material</b> Titanium alloy/POM	K2109.3800	3.8 mm
		K2109.4300	4.3 mm
		K2109.5000	5.0 mm
		K2109.6000	6.0 mm
	<b>Impression caps for impression post, closed tray</b> (5 units)  <b>Material</b> POM	J2111.3300	3.3 mm
		J2111.3800	3.8 mm
		J2111.4300	4.3 mm
		J2111.5000	5.0 mm
		J2111.6000	6.0 mm

## Bite registration

Article	Art. No.	$\varnothing$
 <p><b>CAMLOG® Bite registration posts</b> incl. fixing screw and bite registration cap (also for Platform Switching)</p> <p><b>Material</b> Titanium alloy/POM</p>	J2140.3300	3.3 mm
	J2140.3800	3.8 mm
	J2140.4300	4.3 mm
	J2140.5000	5.0 mm
	J2140.6000	6.0 mm
 <p><b>Bite registration caps</b> (5 units)</p> <p><b>Material</b> POM</p>	J2112.3300	3.3 mm
	J2112.3800	3.8 mm
	J2112.4300	4.3 mm
	J2112.5000	5.0 mm
	J2112.6000	6.0 mm

## Fabrication of the plaster model

Article	Art. No.	$\varnothing$
 <p><b>CAMLOG® Lab analog</b> for cast models</p> <p><b>Material</b> Titanium alloy</p>	K3010.3300	3.3 mm
	K3010.3800	3.8 mm
	K3010.4300	4.3 mm
	K3010.5000	5.0 mm
	K3010.6000	6.0 mm
 <p><b>CAMLOG® Implant analog</b> for printed and cast models</p> <p><b>Material</b> Titanium alloy</p>	K3025.3300	3.3 mm
	K3025.3800	3.8 mm
	K3025.4300	4.3 mm
	K3025.5000	5.0 mm
	K3025.6000	6.0 mm
 <p><b>DIM Analog® for the CAMLOG® Implant System</b> for printed models, incl. thumbscrew</p> <p><b>Material</b> Titanium alloy/Stainless steel</p>	K3012.3300	3.3 mm
	K3012.3800	3.8 mm
	K3012.4300	4.3 mm
	K3012.5000	5.0 mm
	K3012.6000	6.0 mm

Manufacturer DIM Analog®: nt-trading GmbH & Co. KG, G.-Braun-Straße 18, 76187 Karlsruhe, Germany

DIM Analog® is a registered trademark of nt-trading GmbH & Co. KG

## Temporary restoration

	Article	Art. No.	$\emptyset$	GH
	CAMLOG® Temporary abutments, PEEK preparable, incl. abutment screw  Material PEEK	K2241.3800 K2241.4300 K2241.5000 K2241.6000	3.8 mm 4.3 mm 5.0 mm 6.0 mm	-
	CAMLOG® Temporary abutments PS, PEEK, for Platform Switching preparable, incl. abutment screw  Material PEEK	K2208.3800 K2208.4300 K2208.5000 K2208.6000	3.8 mm 4.3 mm 5.0 mm 6.0 mm	-
	CAMLOG® Temporary abutment, crown, titanium alloy incl. abutment screw  Material Titanium alloy	K2239.3300 K2239.3800 K2239.4300 K2239.5000 K2239.6000	3.3 mm* 3.8 mm 4.3 mm 5.0 mm 6.0 mm	-
	CAMLOG® Temporary abutment, bridge, titanium alloy incl. abutment screw  Material Titanium alloy	J2339.3300 J2339.3800 J2339.4300 J2339.5000 J2339.6000	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm	-

## Esthomic® Abutments

Cemented crown and bridge restorations

	Article	Art. No.	$\emptyset$	GH
	CAMLOG® Esthomic® Abutments, straight preparable, incl. abutment screw  Material Titanium alloy	K2226.3810 K2226.3830 K2226.4310 K2226.4330 K2226.5010 K2226.5030 K2226.6010 K2226.6030	3.8 mm 3.8 mm 4.3 mm 4.3 mm 5.0 mm 5.0 mm 6.0 mm 6.0 mm	1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm
	CAMLOG® Esthomic® Abutments, 15° angled, type A preparable, incl. abutment screw  Material Titanium alloy	K2227.3810 K2227.3830 K2227.4310 K2227.4330 K2227.5010 K2227.5030 K2227.6010 K2227.6030	3.8 mm 3.8 mm 4.3 mm 4.3 mm 5.0 mm 5.0 mm 6.0 mm 6.0 mm	1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm

CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

	Article	Art. No.	$\emptyset$	GH
	<b>CAMLOG® Esthomic® Abutments, 15° angled, type B preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2228.3810 K2228.3830 K2228.4310 K2228.4330 K2228.5010 K2228.5030 K2228.6010 K2228.6030	3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm
	<b>CAMLOG® Esthomic® Abutments, 20° angled, type A preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2231.3810 K2231.3830 K2231.4310 K2231.4330 K2231.5010 K2231.5030 K2231.6010 K2231.6030	3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm
	<b>CAMLOG® Esthomic® Abutments, 20° angled, type B preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2232.3810 K2232.3830 K2232.4310 K2232.4330 K2232.5010 K2232.5030 K2232.6010 K2232.6030	3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm 1.0 – 1.8 mm 3.0 – 4.5 mm
	<b>CAMLOG® Esthomic® Abutments, Inset preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2235.3315 K2235.3815 K2235.4315 K2235.5015 K2235.6015	3.3 mm* 3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.5 – 2.8 mm
	<b>CAMLOG® Esthomic® Abutments PS, straight, for Platform Switching preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2202.3815 K2202.4315 K2202.5015 K2202.6015	3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.5 – 2.5 mm
	<b>CAMLOG® Esthomic® Abutments PS, 15° angled, type A, for Platform Switching preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2203.3815 K2203.4315 K2203.5015 K2203.6015	3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.5 – 2.5 mm
	<b>CAMLOG® Esthomic® Abutments PS, 15° angled, type B, for Platform Switching preivable, incl. abutment screw</b> <b>Material</b> Titanium alloy	K2204.3815 K2204.4315 K2204.5015 K2204.6015	3.8 mm 4.3 mm 5.0 mm 6.0 mm	1.5 – 2.5 mm

CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

# CAD/CAM prosthetics

## Crown, bridge and hybrid restorations

	Article	Art. No.	$\emptyset$	GH
	<b>CAMLOG® Titanium bases CAD/CAM, crown</b> bonding base for individual CAD/CAM fabricated dental prosthesis, incl. abutment screw and bonding aid (POM)	K2244.3348	3.3 mm*	
	<b>Material</b> Titanium alloy/POM	K2244.3848	3.8 mm	
		K2244.4348	4.3 mm	-
		K2244.5048	5.0 mm	
		K2244.6048	6.0 mm	
	<b>CAMLOG® Titanium bases CAD/CAM, bridge</b> bonding base for individual CAD/CAM fabricated dental prosthesis, incl. abutment screw and bonding aid (POM)	J2344.3348	3.3 mm	
	<b>Material</b> Titanium alloy/POM	J2344.3848	3.8 mm	
		J2344.4348	4.3 mm	-
		J2344.5048	5.0 mm	
		J2344.6048	6.0 mm	
	<b>CAMLOG® Titanium base CAD/CAM PS for Platform Switching, crown</b> bonding base for individual CAD/CAM fabricated dental prosthesis, incl. abutment screw and bonding aid (POM)	K2210.3808	3.8 mm	
	<b>Material</b> Titanium alloy/POM	K2210.4308	4.3 mm	0.8 mm
		K2210.5008	5.0 mm	

The geometries of the CAMLOG® Titanium bases CAD/CAM are available as a CAD library for leading dental CAD systems. The libraries are available for free download at: [www.camlog.com/en/media-center/cad-libraries](http://www.camlog.com/en/media-center/cad-libraries).

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

### DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® products at your appropriate Camlog country representative.

	Article	Art. No.	$\emptyset$
 11 mm	<b>CAMLOG® Modeling aids for CAMLOG® Titanium bases CAD/CAM burn-out, for fabricating mesostructures and crowns</b>	J2244.3302	3.3 mm
	<b>Material</b> POM	J2244.3802	3.8 mm
		J2244.4302	4.3 mm
		J2244.5002	5.0 mm
		J2244.6002	6.0 mm
 10 mm	<b>CAMLOG® Scanbodies**</b> for optical, 3-dimensional localization of CAMLOG® Implants in the mouth or CAMLOG® Lab analogs in the working model, incl. abutment screw, sterile	K2610.3310	3.3 mm
	Not compatible with the CEREC and inLab systems from Sirona®	K2610.3810*	3.8 mm
	<b>Material</b> PEEK	K2610.4310*	4.3 mm
		K2610.6010*	5.0 mm
			6.0 mm
 10.2 mm	<b>CAMLOG® ScanPosts for Sirona® Scanbody</b> for digital recording of the CAMLOG® Implant or lab analog position and for further processing in the Sirona® CEREC and inLab systems, incl. abutment screw	K2620.3306	3.3 mm
	<b>Material</b> Titanium alloy	K2620.3806*	3.8 mm
		K2620.4306*	4.3 mm
		K2620.5006*	5.0 mm
		K2620.6006*	6.0 mm

\*\* Please check whether the CAMLOG® Scanbody is available in the CAD software used. CAD libraries for selected CAMLOG® Prosthetic components are available for free download at:  
[www.camlog.com/en/media-center/cad-libraries](http://www.camlog.com/en/media-center/cad-libraries).

#### Matching Sirona® Scanbodies size S for CAMLOG® ScanPosts and CAMLOG® Titanium base CAD/CAM crown with $\emptyset$ 3.3/3.8/4.3 mm:

For Omnicam®: Article number 6431311      For Bluecam®: Article number 6431295

#### Matching Sirona® Scanbodies size L for CAMLOG® ScanPosts and CAMLOG® Titanium base CAD/CAM crown with $\emptyset$ 5.0/6.0 mm:

For Omnicam®: Article number 6431329      For Bluecam®: Article number 6431303

Sirona® Scanbodies are available from Dentsply Sirona®.

\* can also be used for Platform Switching

# CAM titanium blanks

Milling production process of individualized one-piece abutments and healing caps by CAD/CAM technology

	Article	Art. No.	$\varnothing$
	<b>CAMLOG® CAM titanium blank, type IAC*</b> $\varnothing$ 12 mm, length 12.5 mm (2 units), sent with 2 separate packed abutment screws	K2411.3313	3.3 mm
	<b>Material</b> Titanium alloy	K2411.3813	3.8 mm
		K2411.4313	4.3 mm
		K2411.6013	5.0 mm
			6.0 mm
	<b>CAMLOG® CAM titanium blank, type ME**</b> $\varnothing$ 12 mm, length 20 mm (2 units), sent with 2 separate packed abutment screws	K2421.3320	3.3 mm
	<b>Material</b> Titanium alloy	K2421.3820	3.8 mm
		K2421.4320	4.3 mm
		K2421.5020	5.0 mm
		K2421.6020	6.0 mm

## Accessories for CAM titanium blanks, type IAC

	Article	Art. No.	$\varnothing$
	<b>CAMLOG® Collet for CAM blank, type IAC*</b> $\varnothing$ 6 mm, length 17 mm, incl. 2 fixing screws for CAM blank, type IAC	K3720.3300	3.3 mm
	<b>Material</b> Stainless steel	K3720.3800	3.8 mm
		K3720.4300	4.3 mm
		K3720.6000	5.0 mm
			6.0 mm

### Type IAC\*

For the milling process, the CAM titanium blank type IAC is fixated to the Implant-abutment connection via the CAMLOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.

### Type ME\*\*

For the milling process, the CAM titanium blank type ME is fixated with the front-facing groove of its cylindrical section via a milling holder for PreFace® Abutments from Medentika®. These milling holders are available for selected machines from the particular machine manufacturer.

The CAM titanium blanks require product specific CAM libraries which are available on request for selected CAM softwares from the software provider.

The geometries of the CAMLOG® CAM titanium blanks are available as a CAD library for leading dental CAD systems. The libraries are available for free download at:

[www.camlog.com/en/media-center/cad-libraries](http://www.camlog.com/en/media-center/cad-libraries).

Medentika® and Preface® are registered trademarks of Medentika GmbH, D-Hügelsheim.

# Universal abutments

## Cemented crown and bridge restorations

	Article	Art. No.	$\emptyset$	Dimension
	<b>CAMLOG® Universal abutments</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	K2211.3300	3.3 mm*	-
		K2211.3800	3.8 mm	
		K2211.4300	4.3 mm	
		K2211.5000	5.0 mm	
		K2211.6000	6.0 mm	
	<b>CAMLOG® Universal abutments PS</b> for Platform Switching preparable, incl. abutment screw  <b>Material</b> Titanium alloy	K2201.3800	3.8 mm	-
		K2201.4300	4.3 mm	
		K2201.5000	5.0 mm	
		K2201.6000	6.0 mm	

# Gold-plastic abutment

## Cemented crown and bridge restorations

	Article	Art. No.	$\emptyset$	Noble metal weight
	<b>CAMLOG® Gold-plastic abutment</b> cast-on, incl. abutment screw  <b>Material</b> Cast-on gold alloy/POM	K2246.3300	3.3 mm*	ca. 0.42 g
		K2246.3800	3.8 mm	ca. 0.46 g
		K2246.4300	4.3 mm	ca. 0.65 g
		K2246.5000	5.0 mm	ca. 0.81 g
		K2246.6000	6.0 mm	ca. 0.89 g

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors ( $\emptyset$  3.3 mm not for double crown restorations)

# Logfit® Prosthetic system

## Cemented crown and bridge restorations

	Article	Art. No.	$\varnothing$	GH
	<b>CAMLOG® Logfit® Abutments</b> incl. abutment screw  <b>Material</b> Titanium alloy	K2550.3808	3.8 mm	0.8 mm
		K2550.3815		1.5 mm
		K2550.4308		0.8 mm
		K2550.4315	4.3 mm	1.5 mm
		K2550.5008	5.0 mm	0.8 mm
		K2550.5015		1.5 mm
		K2550.6008	6.0 mm	0.8 mm
		K2550.6015		1.5 mm
	<b>Logfit® Impression caps</b>  <b>Material</b> POM	J2551.4300	3.8 mm	-
			4.3 mm	
		J2551.6000	5.0 mm	-
			6.0 mm	
	<b>Logfit® Analog</b>  <b>Material</b> Titanium alloy	J2552.4300	3.8 mm	-
			4.3 mm	
		J2552.6000	5.0 mm	-
			6.0 mm	
	<b>Logfit® Plastic copings, for crowns</b> (with rotation securing device) burn-out  <b>Material</b> POM	J2553.4302	3.8 mm	-
			4.3 mm	
		J2553.6002	5.0 mm	-
			6.0 mm	
	<b>Logfit® Plastic copings, for bridges</b> (without rotation securing device) burn-out  <b>Material</b> POM	J2553.4301	3.8 mm	-
			4.3 mm	
		J2553.6001	5.0 mm	-
			6.0 mm	

# COMFOUR®

## Occlusally screw-retained restorations

	Article	Art. No.	Type	$\emptyset$	GH	PP $\emptyset$
	<b>CAMLOG® Bar abutment, straight sterile</b>  <b>Material</b> Titanium alloy	J2254.3305	-	3.3 mm	0.5 mm	4.3 mm
		J2254.3320			2.0 mm	
		J2254.3805		3.8 mm	0.5 mm	
		J2254.3820			2.0 mm	
		J2254.3840		4.0 mm	4.0 mm	
		J2254.4305			0.5 mm	
		J2254.4320		4.3 mm	2.0 mm	
		J2254.4340			4.0 mm	
		J2254.5005		5.0 mm	0.5 mm	
		J2254.5020			2.0 mm	6.0 mm
		J2254.5040			4.0 mm	
	<b>CAMLOG® Bar abutment, 17° angled incl. light blue anodized abutment screw with reduced head, sterile</b>  <b>Material</b> Titanium alloy	K2256.3325	A	3.3 mm	2.5 mm	4.3 mm
		K2256.3340			4.0 mm	
		K2257.3325			2.5 mm	
		K2257.3340			4.0 mm	
		K2256.3825	A	3.8 mm	2.5 mm	
		K2256.3840			4.0 mm	
		K2257.3825	B	4.3 mm	2.5 mm	
		K2257.3840			4.0 mm	
		K2256.4325	A	5.0 mm	2.5 mm	
		K2256.4340			4.0 mm	
		K2257.4325	B	4.3 mm	2.5 mm	
		K2257.4340			4.0 mm	
		K2256.5025	A	5.0 mm	2.5 mm	6.0 mm
		K2256.5040			4.0 mm	
		K2257.5025	B	5.0 mm	2.5 mm	
		K2257.5040			4.0 mm	
	<b>CAMLOG® Bar abutment, 30° angled incl. light blue anodized abutment screw with reduced head, sterile</b>  <b>Material</b> Titanium alloy	K2258.3325	A	3.3 mm	2.5 mm	4.3 mm
		K2258.3340			4.0 mm	
		K2259.3325			2.5 mm	
		K2259.3340			4.0 mm	
		K2258.3825	A	3.8 mm	2.5 mm	
		K2258.3840			4.0 mm	
		K2259.3825	B	4.3 mm	2.5 mm	
		K2259.3840			4.0 mm	
		K2258.4325	A	5.0 mm	2.5 mm	
		K2258.4340			4.0 mm	
		K2259.4325	B	4.3 mm	2.5 mm	
		K2259.4340			4.0 mm	
		K2258.5035	A	5.0 mm	3.5 mm	6.0 mm
		K2258.5050			5.0 mm	
		K2259.5035	B	5.0 mm	3.5 mm	
		K2259.5050			5.0 mm	

Type A and B see on page 7

# COMFOUR®

## Occlusally screw-retained restorations

	Article	Art. No.	Ø	Dimension
	Orientation gauge for COMFOUR® for Ø 2.0 mm pilot drill hole  Material Nitinol	J3551.0001	-	-
	Aligning tool for angled bar abutments, for insertion post	J2269.0003*	-	17°
		J2269.0004*	-	30°
	Material Stainless steel	J2269.0005**	-	17°
		J2269.0006**	-	30°
	Gingiva height indicator, straight  Material Titanium alloy	J3550.3300	3.3 mm	
		J3550.3800	3.8 mm	
		J3550.4300	4.3 mm	
		J3550.5000	5.0 mm	
	Driver for impression caps and healing caps for bar abutments  Material Stainless steel	J5300.0027	3.3 mm	3.8 mm
		J5300.0028	4.3 mm	5.0 mm
	Healing cap for bar abutment partial light blue anodized, sterile  Material Titanium alloy	J2029.4300	3.3 mm	3.8 mm
		J2029.6000	4.3 mm	5.0 mm
	Impression cap, short, for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile  Material Titanium alloy	J2129.4300	3.3 mm	3.8 mm
		J2129.6000	4.3 mm	5.0 mm
	Impression cap, long, for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile  Material Titanium alloy	J2129.4310	3.3 mm	3.8 mm
		J2129.6010	4.3 mm	5.0 mm
	Bar lab analog for bar abutments  Material Stainless steel	J3020.4300	3.3 mm	3.8 mm
		J3020.6000	4.3 mm	5.0 mm
	Bar Implant analog for bar abutments for printed and cast models  Material Stainless steel	J3025.4300	3.3 mm	3.8 mm
		J3025.6000	4.3 mm	5.0 mm
	Scanning cap for bar abutments incl. prosthetic screw light blue anodized, sterile  Material PEEK	J2610.4300	3.3 mm	3.8 mm
		J2610.6000	4.3 mm	5.0 mm
	Titanium cap for bar abutment, for crown incl. prosthetic screw light blue anodized, sterile  Material Titanium alloy	J2259.4301	3.3 mm	3.8 mm
		J2259.6001	4.3 mm	5.0 mm


\* only for use with CAMLOG® Implants with Art. No. K1032.xxxx, K1042.xxxx, K1052.xxxx and K1053.xxxx.

\*\* only for use with CAMLOG® Implants with Art. No. K1044.xxxx, K1054.xxxx, K1075.xxxx and K1076.xxxx.

	Article	Art. No.	$\varnothing$			Dimension
	Titanium cap for bar abutment, for bridge incl. prosthetic screw light blue anodized, sterile	J2259.4302	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6002	5.0 mm			-
	Titanium cap without retention for bar abutment, for bridge incl. prosthetic screw light blue anodized	J2259.4322	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6022	5.0 mm			-
	Crown base for bar abutment burn-out	J2256.4306	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2256.6006	5.0 mm			-
	Base for bar abutment burn-out	J2257.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2257.6001	5.0 mm			-
	Base for bar abutment cast-on	J2263.4300	3.3 mm	3.8 mm	4.3 mm	ca. 0.48 g
	Material Cast-on gold alloy/POM	J2263.6000	5.0 mm			ca. 0.70 g
	Base for bar abutment solderable	J2258.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Solderable gold alloy	J2258.6000	5.0 mm			-
	Base for bar abutment, titanium laser-weldable	J2262.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titan Grade 4	J2262.6000	5.0 mm			-
	Titanium bonding base for bar abutment Passive-Fit	J2260.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2260.6001	5.0 mm			-
	Bar sleeve for titanium bonding base burn-out, Passive-Fit, incl. prosthetic screw for bar abutments, hex (only for fabrication of the cast framework in conjunction with bar sleeves for titanium bonding base Passive-Fit)	J2261.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2261.6001	5.0 mm			-

# COMFOUR®

## Occlusally screw-retained restorations

	Article	Art. No.	Ø			Thread
	Polishing protection for caps and bases for bar abutment	J3021.4300	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J3021.6000	5.0 mm			M 2.0
	Locator® Fixture for bar abutment	J2253.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy/TiN	J2253.6001	5.0 mm			-
	CAMLOG® Abutment screw with reduced head, hex, light blue anodized	J4004.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4004.2001	5.0 mm			M 2.0
	CAMLOG® Lab screw with reduced head, hex, partial light blue anodized	J4004.1600	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4004.2000	5.0 mm			M 2.0
	Prosthetic screw for bar abutments hex, light blue anodized (for final fixation of the restoration)	J4012.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4012.2001	5.0 mm			M 2.0
	Lab prosthetic screw for bar abutment hex, brown anodized	J4013.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4013.2001	5.0 mm			M 2.0
	Screw, hex, length 10 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1610	-			M 1.6
	Material Titanium alloy	J4012.2010	-			M 2.0
	Screw, hex, length 15 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1615	-			M 1.6
	Material Titanium alloy	J4012.2015	-			M 2.0

Lab screws may not be used on patients.

	Article	Art. No.	$\emptyset$	Thread
	Screw, hex, length 20 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1620	-	M 1.6
	<b>Material</b> Titanium alloy	J4012.2020		M 2.0
	Plastic screw for bar abutment hex, length 27 mm, sterile	J4009.1627	-	M 1.6
	<b>Material</b> PEEK	J4009.2027		M 2.0

## Ball abutment anchoring system

	Article	Art. No.	$\emptyset$	GH
	CAMLOG® Ball abutments, male part incl. stabilizing ring	J2249.3315	3.3 mm	1.5 mm
		J2249.3330		3.0 mm
		J2249.3815	3.8 mm	1.5 mm
		J2249.3830		3.0 mm
		J2249.3845	4.3 mm	4.5 mm
		J2249.4315		1.5 mm
		J2249.4330	4.3 mm	3.0 mm
		J2249.4345		4.5 mm
		J2249.5015	5.0 mm	1.5 mm
		J2249.5030		3.0 mm
		J2249.5045		4.5 mm
	Matrix CM Dalbo®-Plus for ball abutment, incl. lamella retention insert	05003503	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	-

Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Biel, Switzerland.

## Ball abutment anchoring system

	Article	Art. No.	$\emptyset$	GH
	Lamella retention insert for matrix CM Dalbo®-Plus	05003504	3.3 mm	-
	Material Gold alloy		3.8 mm	
			4.3 mm	
			5.0 mm	
	Ball abutment analogs incl. stabilizing ring	J3015.3300	3.3 mm	-
	Material Brass/Plastic	J3015.3800	3.8 mm	
		J3015.4300	4.3 mm	
		J3015.5000	5.0 mm	

## Locator® Anchoring system

CAMLOG® Locator R-Tx®

	Article	Art. No.	$\emptyset$	GH
	CAMLOG® Locator R-Tx® Abutment incl. titanium housing with processing replacement male black, block-out spacer white and four different retention inserts	30800-01	3.3 mm	1.0 mm
	Material Titanium alloy/Nylon	30800-02		2.0 mm
		30800-03		3.0 mm
		30800-04		4.0 mm
	Locator R-Tx® Impression coping (4 units)	30801-01	3.8 mm	1.0 mm
	Material Polyethylene	30801-02		2.0 mm
		30801-03		3.0 mm
		30801-04		4.0 mm
	Locator R-Tx® Analog $\emptyset$ 3.35 mm (4 units)	30801-05	4.3 mm	5.0 mm
	Material Aluminum	30802-01		1.0 mm
		30802-02		2.0 mm
		30802-03		3.0 mm
		30802-04	5.0 mm	4.0 mm
		30802-05		5.0 mm
		30803-01		1.0 mm
		30803-02		2.0 mm
		30803-03		3.0 mm
		30803-04		4.0 mm
		30803-05		5.0 mm
	Locator R-Tx® Analog $\emptyset$ 3.35 mm (4 units)	30017-01	3.3 mm	-
	Material Aluminum		3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator R-Tx® Analog $\emptyset$ 3.35 mm (4 units)	30014-01	3.3 mm	-

	Article	Art. No.	$\emptyset$
	<b>Locator R-Tx® Analog</b> Ø 4.0 mm (4 units) <b>Material</b> Aluminum	30015-01	3.8 mm 4.3 mm
	<b>Locator R-Tx® Analog</b> Ø 5.0 mm (4 units) <b>Material</b> Aluminum	30016-01	5.0 mm
	<b>Locator R-Tx®</b> <b>Titanium housing</b> with processing insert black (4 units) <b>Material</b> Titanium alloy/Polyethylene	30013-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<b>Locator R-Tx®</b> <b>Processing insert</b> black (4 units) <b>Material</b> Polyethylene	30012-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<b>Locator R-Tx®</b> <b>Processing spacer</b> (4 units) <b>Material</b> Polyethylene	30018-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<b>Locator R-Tx®</b> <b>Retention insert</b> gray, ZERO RETENTION (4 units) <b>Material</b> Nylon	30001-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<b>Locator R-Tx®</b> <b>Retention insert</b> blue, LIGHT (4 units) <b>Material</b> Nylon	30002-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm

## Locator® Anchoring system

CAMLOG® Locator R-Tx®

	Article	Art. No.	Ø	GH
	<b>Locator R-Tx®</b> <b>Retention insert</b> pink, MEDIUM (4 units) <b>Material</b> Nylon	30003-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	<b>Locator R-Tx®</b> <b>Retention insert</b> white, STRONG (4 units) <b>Material</b> Nylon	30004-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-

## Locator® Anchoring system

CAMLOG® Locator®

	Article	Art. No.	Ø	GH
	<b>CAMLOG® Locator®</b> <b>Abutment</b> <b>Material</b> Titanium alloy/TiN	J2253.3310 J2253.3320 J2253.3330 J2253.3340 J2253.3810 J2253.3820 J2253.3830 J2253.3840 J2253.3850 J2253.4310 J2253.4320 J2253.4330 J2253.4340 J2253.4350 J2253.5010 J2253.5020 J2253.5030 J2253.5040 J2253.5050	3.3 mm 3.8 mm 4.3 mm 5.0 mm	1.0 mm 2.0 mm 3.0 mm 4.0 mm 1.0 mm 2.0 mm 3.0 mm 4.0 mm 5.0 mm 1.0 mm 2.0 mm 3.0 mm 4.0 mm 5.0 mm 1.0 mm 2.0 mm 3.0 mm 4.0 mm 5.0 mm
	<b>Locator® Impression cap</b> (4 units) <b>Material</b> Aluminum/Polyethylene	J2253.0200	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	<b>Locator® Analog</b> (4 units) <b>Material</b> Aluminum	J2253.0340 J2253.0350	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-

	Article	Art. No.	$\varnothing$
	<p><b>Locator® Male processing package</b> (2 units)</p> <p><b>Content per package:</b> 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male clear 1 Replacement male pink 1 Replacement male blue</p> <p><b>Material</b> Titanium alloy/Polyethylene/Teflon/Nylon</p>	J2253.0102	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<p><b>Locator® Male processing package for extended range</b> (2 units)</p> <p><b>Content per package:</b> 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male green 1 Replacement male orange 1 Replacement male red</p> <p><b>Material</b> Titanium alloy/Polyethylene/Teflon/Nylon</p>	J2253.0112	3.8 mm 4.3 mm 5.0 mm
	<p><b>Locator® Block out spacer</b> (20 units)</p> <p><b>Material</b> Teflon</p>	J2253.0401	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<p><b>Locator® Processing replacement male</b> (4 units)</p> <p><b>Material</b> Polyethylen</p>	J2253.0402	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<p><b>Locator® Replacement male clear, STRONG, Div.: 0°-10°</b> (4 units)</p> <p><b>Material</b> Nylon</p>	J2253.1005	3.3 mm 3.8 mm 4.3 mm 5.0 mm

# Locator® Anchoring system

## CAMLOG® Locator®

	Article	Art. No.	Ø
	<b>Locator® Replacement male</b> pink, MEDIUM, Div.: 0° – 10° (4 units)  <b>Material</b> Nylon	J2253.1003	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<b>Locator® Replacement male</b> blue, LIGHT, Div.: 0° – 10° (4 units)  <b>Material</b> Nylon	J2253.1002	3.3 mm 3.8 mm 4.3 mm 5.0 mm
	<b>Locator® Replacement male</b> for extended range* green, STRONG, Div.: 10° – 20° (4 units)  <b>Material</b> Nylon	J2253.2004	3.8 mm 4.3 mm 5.0 mm
	<b>Locator® Replacement male</b> for extended range* orange, MEDIUM, Div.: 10° – 20° (4 units)  <b>Material</b> Nylon	J2253.2003	3.8 mm 4.3 mm 5.0 mm
	<b>Locator® Replacement male</b> for extended range* red, LIGHT, Div.: 10° – 20° (4 units)  <b>Material</b> Nylon	J2253.2002	3.8 mm 4.3 mm 5.0 mm
	<b>Locator® Replacement male</b> for extended range* gray, NO RETENTION, Div.: 0° – 20° (4 units)  <b>Material</b> Nylon	J2253.2000	3.8 mm 4.3 mm 5.0 mm

\* not permitted for Implant Ø 3.3 mm

Manufacturer Locator®: Zest Anchors, 2875 Loker Avenue East, Carlsbad, California 92010, USA  
Locator® and Locator R-Tx® are a registered trademark of Zest Anchors

# Double crown restorations

	Article	Art. No.	$\varnothing$
 11 mm	<b>CAMLOG® Universal abutments for double crown restorations</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	K2211.3800	3.8 mm
		K2211.4300	4.3 mm
		K2211.5000	5.0 mm
		K2211.6000	6.0 mm
 11 mm	<b>CAMLOG® Universal abutments PS for double crown restorations for Platform Switching</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	K2201.3800	3.8 mm
		K2201.4300	4.3 mm
		K2201.5000	5.0 mm
		K2201.6000	6.0 mm
 12 mm	<b>CAMLOG® Telescope abutments for double crown restorations</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	K2212.3800	3.8 mm
		K2212.4300	4.3 mm
		K2212.5000	5.0 mm
		K2212.6000	6.0 mm

## Accessories for abutments

	Article	Art. No.	$\varnothing$	Thread
	<b>CAMLOG® Abutment screw, hex</b> for definitive screw retention of abutments into the Implant  <b>Material</b> Titanium alloy	J4005.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		J4005.2001	5.0 mm	M 2.0
			6.0 mm	
	<b>CAMLOG® Lab screw, hex</b> for the fixation of abutments on the working model, brown anodized  <b>Material</b> Titanium alloy	J4006.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		J4006.2001	5.0 mm	M 2.0
			6.0 mm	

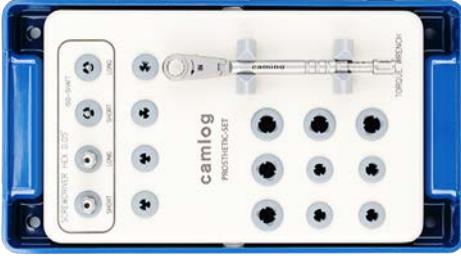
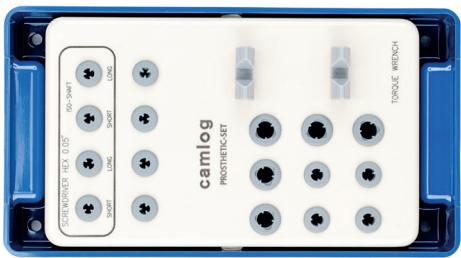
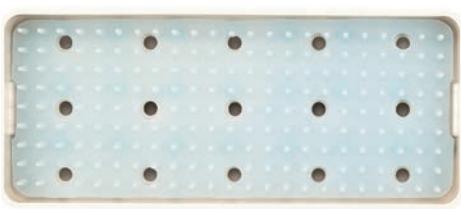
CAMLOG® Abutments PS may only be used on CAMLOG® Implants with a K article number.  
 Lab screws may not be used on patients.

## Prosthetic instruments

	Article	Art. No.	L
	<p><b>Torque wrench</b> with continuous torque adjustment until maximal 30 Ncm</p> <p><b>Material</b> Stainless steel</p>	J5320.1030	-
	<p><b>Driver</b> for ball abutment manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J5300.0011	18.3 mm
	<p><b>Screwdriver Activator</b> for ball abutment matrix CM Dalbo®-Plus</p> <p><b>Material</b> Stainless steel</p>	07000389	-
	<p><b>Driver for straight bar abutment, short</b> Ø 3.3/3.8/4.3 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0020	18.6 mm
	<p><b>Driver for straight bar abutment, short</b> Ø 5.0 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0025	18.6 mm

	Article	Art. No.	L
	<b>Driver for straight bar abutment, long</b> Ø 3.3/3.8/4.3 mm  <b>Material</b> Stainless steel	J5300.0021	28.0 mm
	<b>Driver</b> for impression cap and healing cap for bar abutment Ø 3.3/3.8/4.3 mm  <b>Material</b> Stainless steel	J5300.0027	19.1 mm
	<b>Driver</b> for impression cap and healing cap for bar abutment Ø 5.0 mm  <b>Material</b> Stainless steel	J5300.0028	19.1 mm
	<b>Driver</b> for Locator®, manual/wrench  <b>Material</b> Stainless steel	J2253.0001	24.3 mm
	<b>Locator® Instrument</b> threepart  <b>Material</b> Stainless steel	J2253.0002	83.0 mm
	<b>Locator® Abutment holder sleeve</b> for golden component of the Locator® Instrument (4 units)  <b>Material</b> Polysulfone	08394	-
	<b>Locator® Angle measurement guide</b>  <b>Material</b> Stainless steel	J2253.0003	-
	<b>Locator® Parallel post</b> (4 units)  <b>Material</b> Polyethylene	J2253.0004	-

# Prosthetic instruments

	Article	Art. No.	Dimension
	<b>Locator R-Tx®</b> Retention insert tool with plastic grip <b>Material</b> Stainless steel	30021-01	-
	<b>Prosthetic set</b> Content: - J5320.1030 Torque wrench - J5317.0501 Screwdriver, hex, short, manual/wrench - J5317.0502 Screwdriver, hex, long, manual/wrench - J5317.0504 Screwdriver, hex, short, ISO shaft - J5317.0503 Screwdriver, hex, long, ISO shaft	J5330.8600	197 x 108 x 54 mm
	<b>Prosthetic tray</b> (without content) <b>Material</b> Plastic	J5330.8500	197 x 108 x 54 mm
	<b>Prosthetic tray universal</b> (without content) resterilizable <b>Material</b> Radel®, Silicone	J5330.8700	162 x 73 x 29 mm
	<b>Screwdriver</b> Hex, extra short, manual/wrench <b>Material</b> Stainless steel	J5317.0510	14.5 mm
	<b>Screwdriver</b> Hex, short, manual/wrench <b>Material</b> Stainless steel	J5317.0501	22.5 mm

	Article	Art. No.	L
	<p><b>Screwdriver</b> Hex, long, manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J5317.0502	30.3 mm
	<p><b>Screwdriver</b> Hex, short, ISO shaft</p> <p><b>Material</b> Stainless steel</p>	J5317.0504	18.0 mm
	<p><b>Screwdriver</b> Hex, long, ISO shaft</p> <p><b>Material</b> Stainless steel</p>	J5317.0503	26.0 mm
	<p><b>Manual screwdriver</b> Hex, without wrench head connection</p> <p><b>Material</b> Stainless steel</p>	J5317.0511	23.0 mm
	<p><b>Handle for</b> <b>CAMLOG®/CONELOG®</b> <b>Implant analog</b></p> <p><b>Material</b> Stainless steel</p>	J3025.0010  J3025.0015	3.3 mm  3.8 mm  4.3 mm  5.0 mm  6.0 mm

# Instruments for dental technicians

	Article	Art. No.	$\emptyset$
	<b>Universal holder</b> incl. 2 CAMLOG® Lab screws, hex, and 1 CAMLOG® Abutment collet each for $\emptyset$ 3.3/3.8/4.3/5.0/6.0 mm  <b>Material</b> Stainless steel/Titanium alloy	J3709.0010	-
	<b>Universal holder</b>  <b>Material</b> Stainless steel	J3709.0015	-
	<b>CAMLOG® Abutment collets</b> for universal holder, for grinding CAMLOG® Abutments  <b>Material</b> Titanium alloy	J3709.3300 J3709.3800 J3709.4300 J3709.5000 J3709.6000	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm
	<b>Reamers for dilating the plaster model,</b> <b>for universal holder</b> incl. color-coded guide pin  <b>Material</b> Stainless steel/Titanium alloy	J3706.3300 J3706.3800 J3706.4300 J3706.5000 J3706.6000	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm
	<b>Reworking reamer,</b> <b>for base for bar abutment</b> plane surface/cone seat, burn-out  <b>Material</b> Stainless steel/Brass	J3711.0010  J3711.0015	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm
	<b>Reworking reamer,</b> <b>for base for bar abutment</b> screw seat, burn-out  <b>Material</b> Stainless steel/Brass	J3711.0020  J3711.0025	3.3 mm 3.8 mm 4.3 mm 5.0 mm 6.0 mm

# Selection abutments

Article	Art. No.
	<b>CAMLOG® Selection abutment kit</b> (Content: 2 units each, according table below)  K8011.1000

Content: CAMLOG® Selection abutment kit					
Article	Material	Ø	Ø	GH	
CAMLOG® Esthomic® Selection abutment, straight*	POM	3.8 mm	4.3 mm	5.0 mm	1.0 – 1.8
CAMLOG® Esthomic® Selection abutment, 15° angled, type A*					3.0 – 4.5
CAMLOG® Esthomic® Selection abutment, 15° angled, type B*					1.0 – 1.8
CAMLOG® Esthomic® Selection abutment, 20° angled, type A*					
CAMLOG® Esthomic® Selection abutment, 20° angled, type B*					

**Attention, do not use selection abutments on patients!**

\* These products are not available singly.





## Implants for practice

	Article	Art. No.	Ø	L
	<b>CAMLOG® PROGRESSIVE-LINE</b> <b>Implant for practice</b> incl. snap-in insertion post and cover screw, yellow anodized  <b>Material</b> Titanium alloy	K1901.3813	3.8 mm	
	<b>CAMLOG® PROGRESSIVE-LINE</b> <b>Implant for practice</b> incl. snap-in insertion post and cover screw, red anodized  <b>Material</b> Titanium alloy	K1901.4313	4.3 mm	13 mm
	<b>CAMLOG® SCREW-LINE</b> <b>Implant for practice</b> incl. insertion post and cover screw, yellow anodized  <b>Material</b> Titanium alloy	K1049.3813	3.8 mm	
	<b>CAMLOG® SCREW-LINE</b> <b>Implant for practice</b> incl. insertion post and cover screw, red anodized  <b>Material</b> Titanium alloy	K1049.4313	4.3 mm	13 mm

Attention, do not use Implants for practice on patients!

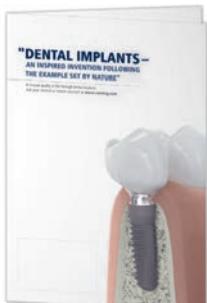
## Demonstration models

	Article	Art. No.
	<p><b>CAMLOG® Demonstration model, acrylic glass</b> upper jaw, 4 CAMLOG® SCREW-LINE Implants, 4 x Ø 4.3 mm</p> <p><b>Material</b> Acrylic glass/Titanium</p>	K8070.1020
	<p><b>CAMLOG® Demonstration model, acrylic glass</b> lower jaw, 4 CAMLOG® SCREW-LINE Implants, 4 x Ø 4.3 mm</p> <p><b>Material</b> Acrylic glass/Titanium</p>	K8050.1040
	<p><b>Edentulous mandible</b> incl. mounting plate</p> <p><b>Material</b> Plastic</p>	J8070.2050

## Macro models

	Article	Art. No.
	<p><b>CAMLOG® PROGRESSIVE-LINE Macro model</b> Scale 3:1</p> <p><b>Content:</b> 1 CAMLOG® PROGRESSIVE-LINE Implant 1 CAMLOG® Esthomic® Abutment, straight 1 CAMLOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CAMLOG® Esthomic® Abutment, straight 1 Acrylic socket</p> <p><b>Material</b> Plastic/Stainless steel</p>	K8010.1400
	<p><b>CAMLOG® SCREW-LINE Macro model</b> Scale 3:1</p> <p><b>Content:</b> 1 CAMLOG® SCREW-LINE Implant 1 CAMLOG® Esthomic® Abutment, straight 1 CAMLOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CAMLOG® Esthomic® Abutment, straight 1 Acrylic socket</p> <p><b>Material</b> Plastic/Stainless steel</p>	K8010.1010


# Literature

	Article	Art. No.
	<b>Patient brochure</b> Questions and answers to dental Implants	-
	<b>COMFOUR® Patient brochure</b> Bridge instead of dentures – dental prosthesis with feel-good factor	-
	<b>Implant pass</b> Patient-specific documentation of Implant restoration Packaging units: 10 units	-
	<b>Patient advice sheets</b> Set á 5 sheets, A4	-
	<b>Presentation folder</b> A4, laminated	-

	Article	Art. No.
	<p><b>Poster</b>            Format: 50 x 70 cm</p>	
	<p><b>Appointment pad</b>            50 sheets/pad, A7            Packaging units: 5 units</p>	

# Indication overview

Single tooth restoration		Bridge restoration
Cemented	Screwed	Cemented
		
Temporary abutments, PEEK, incl. PS	Temporary abutments, PEEK, incl. PS	Temporary abutments, PEEK, incl. PS
		
	Temporary abutment, crown, titanium alloy	
		
Esthomic® Abutments, incl. PS		Esthomic® Abutments, incl. PS
		
	Bar abutments	
		
Titanium bases CAD/CAM, crown, incl. PS	Titanium bases CAD/CAM, crown, incl. PS	Titanium bases CAD/CAM, bridge
		
Logfit® Abutment		Logfit® Abutment
		
Universal abutment, CAM titanium blank incl. PS		Universal abutment, CAM titanium blank incl. PS
		
Gold-plastic abutment	Gold-plastic abutment	Gold-plastic abutment

Bridge restoration	Hybrid restoration
Screwed	Removable (full denture)
 Temporary abutment, crown, titanium alloy	
 Bar abutments	 Bar abutments
 Titanium bases CAD/CAM, bridge	 Locator® Anchoring system
	 Ball abutment
	 Universal abutment, incl. PS
	 CAM titanium blank
Double crown restoration	 Telescope abutment
	 Gold-plastic abutment
	 Titanium bases CAD/CAM, crown, incl. PS



# Implant overview

Article		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	L
		Art. No. A Ø				
	-	K1076.3809 A Ø 3.0 mm	K1076.4309 A Ø 3.0 mm	K1076.5009 A Ø 3.5 mm	9 mm	
	K1076.3311 A Ø 2.2 mm	K1076.3811 A Ø 2.7 mm	K1076.4311 A Ø 2.7 mm	K1076.5011 A Ø 3.2 mm	11 mm	
	K1076.3313 A Ø 2.2 mm	K1076.3813 A Ø 2.7 mm	K1076.4313 A Ø 2.7 mm	K1076.5013 A Ø 3.2 mm	13 mm	
	K1076.3316 A Ø 2.2 mm	K1076.3816 A Ø 2.7 mm	K1076.4316 A Ø 2.7 mm	K1076.5016 A Ø 3.2 mm	16 mm	
	-	K1075.3809 A Ø 3.0 mm	K1075.4309 A Ø 3.0 mm	K1075.5009 A Ø 3.5 mm	9 mm	
	K1075.3311 A Ø 2.2 mm	K1075.3811 A Ø 2.7 mm	K1075.4311 A Ø 2.7 mm	K1075.5011 A Ø 3.2 mm	11 mm	
	K1075.3313 A Ø 2.2 mm	K1075.3813 A Ø 2.7 mm	K1075.4313 A Ø 2.7 mm	K1075.5013 A Ø 3.2 mm	13 mm	
	K1075.3316 A Ø 2.2 mm	K1075.3816 A Ø 2.7 mm	K1075.4316 A Ø 2.7 mm	K1075.5016 A Ø 3.2 mm	16 mm	

Article		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	L
		A Ø 2.7 mm	A Ø 3.5 mm	A Ø 3.9 mm	A Ø 4.6 mm	A Ø 5.5 mm	
	-	K1046.3809	K1046.4309	K1046.5009	K1046.6009	9 mm	
	K1046.3311	K1046.3811	K1046.4311	K1046.5011	K1046.6011	11 mm	
	K1046.3313	K1046.3813	K1046.4313	K1046.5013	K1046.6013	13 mm	
	K1046.3316	K1046.3816	K1046.4316	K1046.5016	K1046.6016	16 mm	
	-	K1045.3809	K1045.4309	K1045.5009	-	9 mm	
	K1045.3311	K1045.3811	K1045.4311	K1045.5011	-	11 mm	
	K1045.3313	K1045.3813	K1045.4313	K1045.5013	-	13 mm	
	K1045.3316	K1045.3816	K1045.4316	-	-	16 mm	
	-	K1056.3809	K1056.4309	K1056.5009	K1056.6009	9 mm	
	K1056.3311	K1056.3811	K1056.4311	K1056.5011	K1056.6011	11 mm	
	K1056.3313	K1056.3813	K1056.4313	K1056.5013	K1056.6013	13 mm	
	K1056.3316	K1056.3816	K1056.4316	K1056.5016	K1056.6016	16 mm	
	-	K1055.3809	K1055.4309	K1055.5009	-	9 mm	
	K1055.3311	K1055.3811	K1055.4311	K1055.5011	-	11 mm	
	K1055.3313	K1055.3813	K1055.4313	K1055.5013	-	13 mm	
	K1055.3316	K1055.3816	K1055.4316	-	-	16 mm	



# Prosthetics overview

## Impression taking

Article	$\varnothing$ 3.3 mm	$\varnothing$ 3.8 mm	$\varnothing$ 4.3 mm	$\varnothing$ 5.0 mm	$\varnothing$ 6.0 mm	GH
 CAMLOG® Impression posts, open tray	K2121.3300	K2121.3800	K2121.4300	K2121.5000	K2121.6000	-
 CAMLOG® Impression posts, closed tray	K2110.3300	K2110.3800	K2110.4300	K2110.5000	K2110.6000	-
  CAMLOG® Impression posts PS, open tray, for Platform Switching with CAMLOG® Implants with K article number	-	K2119.3800	K2119.4300	K2119.5000	K2119.6000	-
  CAMLOG® Impression posts PS, closed tray, for Platform Switching with CAMLOG® Implants with K article number	-	K2109.3800	K2109.4300	K2109.5000	K2109.6000	-
 Impression caps for impression post, closed tray	J2111.3300	J2111.3800	J2111.4300	J2111.5000	J2111.6000	-

## Bite registration

 CAMLOG® Bite registration posts incl. fixing screw and bite registration cap	J2140.3300	J2140.3800	J2140.4300	J2140.5000	J2140.6000	-
--	------------	------------	------------	------------	------------	---

## Fabrication of the plaster model

 CAMLOG® Lab analogs, for cast models	K3010.3300	K3010.3800	K3010.4300	K3010.5000	K3010.6000	-
 CAMLOG® Implant analogs, for printed and cast models	K3025.3300	K3025.3800	K3025.4300	K3025.5000	K3025.6000	-
 DIM Analog® for printed models for the CAMLOG® Implant System	K3012.3300	K3012.3800	K3012.4300	K3012.5000	K3012.6000	-

## Abutments for crown and bridge restorations

Article	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	GH	
	CAMLOG® Temporary abutments, PEEK	-	K2241.3800	K2241.4300	K2241.5000	K2241.6000	-
	CAMLOG® Temporary abutments PS, PEEK, for Platform Switching with CAMLOG® Implants with K article number	-	K2208.3800	K2208.4300	K2208.5000	K2208.6000	-
	CAMLOG® Temporary abutments, crown, titanium alloy	K2239.3300	K2239.3800	K2239.4300	K2239.5000	K2239.6000	-
	CAMLOG® Temporary abutments, bridge, titanium alloy	J2339.3300	J2339.3800	J2339.4300	J2339.5000	J2339.6000	-
	CAMLOG® Esthomic® Abutments, straight	-	K2226.3810	K2226.4310	K2226.5010	K2226.6010	1.0-1.8 mm
			K2226.3830	K2226.4330	K2226.5030	K2226.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 15° angled, type A	-	K2227.3810	K2227.4310	K2227.5010	K2227.6010	1.0-1.8 mm
			K2227.3830	K2227.4330	K2227.5030	K2227.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 15° angled, type B	-	K2228.3810	K2228.4310	K2228.5010	K2228.6010	1.0-1.8 mm
			K2228.3830	K2228.4330	K2228.5030	K2228.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 20° angled, type A	-	K2231.3810	K2231.4310	K2231.5010	K2231.6010	1.0-1.8 mm
			K2231.3830	K2231.4330	K2231.5030	K2231.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments, 20° angled, type B	-	K2232.3810	K2232.4310	K2232.5010	K2232.6010	1.0-1.8 mm
			K2232.3830	K2232.4330	K2232.5030	K2232.6030	3.0-4.5 mm
	CAMLOG® Esthomic® Abutments PS, straight, for Platform Switching with CAMLOG® Implants with K article number	-	K2202.3815	K2202.4315	K2202.5015	K2202.6015	1.5 - 2.5 mm
	CAMLOG® Esthomic® Abutments PS, 15° angled, type A, for Platform Switching with CAMLOG® Implants with K article number	-	K2203.3815	K2203.4315	K2203.5015	K2203.6015	1.5 - 2.5 mm
	CAMLOG® Esthomic® Abutments PS, 15° angled, type B, for Platform Switching with CAMLOG® Implants with K article number	-	K2204.3815	K2204.4315	K2204.5015	K2204.6015	1.5 - 2.5 mm

# Prosthetics overview

## Abutments for crown and bridge restorations

Article	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	GH
 CAMLOG® Esthomic® Abutments, Inset	K2235.3315	K2235.3815	K2235.4315	K2235.5015	K2235.6015	1.5 – 2.5 mm
 CAMLOG® Universal abutments	K2211.3300	K2211.3800	K2211.4300	K2211.5000	K2211.6000	-
 CAMLOG® Universal abutments PS for Platform Switching with CAMLOG® Implants with K article number	-	K2201.3800	K2201.4300	K2201.5000	K2201.6000	-
 CAMLOG® Gold-plastic abutments	K2246.3300	K2246.3800	K2246.4300	K2246.5000	K2246.6000	-
 CAMLOG® Titanium bases CAD/CAM, crown	K2244.3348	K2244.3848	K2244.4348	K2244.5048	K2244.6048	-
 CAMLOG® Titanium bases CAD/CAM PS, crown	-	K2210.3808	K2210.4308	K2210.5008	-	0.8 mm
 CAMLOG® Titanium bases CAD/CAM, bridge	J2344.3348	J2344.3848	J2344.4348	J2344.5048	J2344.6048	-
 CAMLOG® Logfit® Abutments	-	K2550.3808	K2550.4308	K2550.5008	K2550.6008	0.8 mm
		K2550.3815	K2550.4315	K2550.5015	K2550.6015	1.5 mm
 Logfit® Impression caps	-	J2551.4300	J2551.4300	J2551.6000	J2551.6000	-
 Logfit® Analog	-	J2552.4300	J2552.4300	J2552.6000	J2552.6000	-
 Logfit® Plastic copings, for crowns	-	J2553.4302	J2553.4302	J2553.6002	J2553.6002	-
 Logfit® Plastic copings, for bridges	-	J2553.4301	J2553.4301	J2553.6001	J2553.6001	-

## COMFOUR® – Abutments for crown, bridge and hybrid restorations

 CAMLOG® Bar abutment, straight	J2254.3305	J2254.3805	J2254.4305	J2254.5005	-	0.5 mm
	J2254.3320	J2254.3820	J2254.4320	J2254.5020		2.0 mm
	-	J2254.3840	J2254.4340	J2254.5040		4.0 mm

Article	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	GH
	Art. No.				
 CAMLOG® Bar abutment, 17° angled, type A	K2256.3325	K2256.3825	K2256.4325	K2256.5025	2.5 mm
	K2256.3340	K2256.3840	K2256.4340	K2256.5040	4.0 mm
 CAMLOG® Bar abutment, 17° angled, type B	K2257.3325	K2257.3825	K2257.4325	K2257.5025	2.5 mm
	K2257.3340	K2257.3840	K2257.4340	K2257.5040	4.0 mm
 CAMLOG® Bar abutment, 30° angled, Type A	K2258.3325	K2258.3825	K2258.4325	K2258.5035*	2.5 mm/3.5 mm*
	K2258.3340	K2258.3840	K2258.4340	K2258.5050*	4.0 mm/5.0 mm*
 CAMLOG® Bar abutment, 30° angled, Type B	K2259.3325	K2259.3825	K2259.4325	K2259.5035*	2.5 mm/3.5 mm*
	K2259.3340	K2259.3840	K2259.4340	K2259.5050*	4.0 mm/5.0 mm*
	J2029.4300	J2029.4300	J2029.4300	J2029.6000	-
	J2129.4300	J2129.4300	J2129.4300	J2129.6000	-
	J2129.4310	J2129.4310	J2129.4310	J2129.6010	-
	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-
	J2259.4301	J2259.4301	J2259.4301	J2259.6001	-
	J2259.4302	J2259.4302	J2259.4302	J2259.6002	-
	J2259.4322	J2259.4322	J2259.4322	J2259.6022	-
	J2256.4306	J2256.4306	J2256.4306	J2256.6006	-
	J2257.4301	J2257.4301	J2257.4301	J2257.6001	-
	J2263.4300	J2263.4300	J2263.4300	J2263.6000	-
	J2258.4300	J2258.4300	J2258.4300	J2258.6000	-
	J2262.4300	J2262.4300	J2262.4300	J2262.6000	-
	J2260.4301	J2260.4301	J2260.4301	J2260.6001	-
	J2261.4301	J2261.4301	J2261.4301	J2261.6001	-
	J2253.4301	J2253.4301	J2253.4301	J2253.6001	-

# Prosthetics overview

## Hybrid restoration

Article	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	GH
Art. No.					
 CAMLOG® Ball abutments, male part	J2249.3315	J2249.3815	J2249.4315	J2249.5015	1.5 mm
	J2249.3330	J2249.3830	J2249.4330	J2249.5030	3.0 mm
	-	J2249.3845	J2249.4345	J2249.5045	4.5 mm
 Matrix CM Dalbo®-Plus	05003503	05003503	05003503	05003503	-
 Ball abutment analogs	J3015.3300	J3015.3800	J3015.4300	J3015.5000	-
 CAMLOG® Locator R-Tx® Abutment	30800-01	30801-01	30802-01	30803-01	1.0 mm
	30800-02	30801-02	30802-02	30803-02	2.0 mm
	30800-03	30801-03	30802-03	30803-03	3.0 mm
	30800-04	30801-04	30802-04	30803-04	4.0 mm
	-	30801-05	30802-05	30803-05	5.0 mm
 Locator R-Tx® Impression coping	30017-01	30017-01	30017-01	30017-01	-
 Locator R-Tx® Analog	30014-01	30015-01	30015-01	30016-01	-
 Locator R-Tx® Titanium housing	30013-01	30013-01	30013-01	30013-01	-
 Locator R-Tx® Processing insert	30012-01	30012-01	30012-01	30012-01	-
 Locator R-Tx® Processing spacer	30018-01	30018-01	30018-01	30018-01	-
 Locator R-Tx® Retention insert gray, ZERO RETENTION	30001-01	30001-01	30001-01	30001-01	-
 Locator R-Tx® Retention insert blue, LIGHT	30002-01	30002-01	30002-01	30002-01	-
 Locator R-Tx® Retention insert pink, MEDIUM	30003-01	30003-01	30003-01	30003-01	-
 Locator R-Tx® Retention insert white, STRONG	30004-01	30004-01	30004-01	30004-01	-
 CAMLOG® Locator® Abutments	J2253.3310	J2253.3810	J2253.4310	J2253.5010	1.0 mm
	J2253.3320	J2253.3820	J2253.4320	J2253.5020	2.0 mm
	J2253.3330	J2253.3830	J2253.4330	J2253.5030	3.0 mm
	J2253.3340	J2253.3840	J2253.4340	J2253.5040	4.0 mm
	-	J2253.3850	J2253.4350	J2253.5050	5.0 mm
 Locator® Impression cap	J2253.0200	J2253.0200	J2253.0200	J2253.0200	-
 Locator® Analog	J2253.0340	J2253.0340	J2253.0340	J2253.0350	-
 Locator® Male processing package	J2253.0102	J2253.0102	J2253.0102	J2253.0102	-
 Locator® Male processing package for extended range	-	J2253.0112	J2253.0112	J2253.0112	-

Article		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	GH
	CAMLOG® Universal abutments	-	K2211.3800	K2211.4300	K2211.5000	K2211.6000	-
	CAMLOG® Universal abutments PS for Platform Switching with CAMLOG® Implants with K article number	-	K2201.3800	K2201.4300	K2201.5000	K2201.6000	-
	CAMLOG® Telescope abutments	-	K2212.3800	K2212.4300	K2212.5000	K2212.6000	-

## CAD/CAM prosthetics

	CAMLOG® Scanbodies	K2610.3310	K2610.3810	K2610.4310	K2610.6010	K2610.6010	-
	CAMLOG® ScanPost for Sirona® Scanbody	K2620.3306	K2620.3806	K2620.4306	K2620.5006	K2620.6006	-
	CAMLOG® CAM titanium blank, type IAC	K2411.3313	K2411.3813	K2411.4313	K2411.6013	K2411.6013	-
	CAMLOG® CAM titanium blank, type ME	K2421.3320	K2421.3820	K2421.4320	K2421.5020	K2421.6020	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-	-

## DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

# Screw overview Abutment and prosthetic screws – intraoral use

## Implant-Abutment connection

Article	CAMLOG® Abutment screw					Tightening torque
	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	
 Temporary abutments PEEK, incl. PS Scanbody ScanPost for Sirona® Scanbody		M 1.6		M 2.0		tightened by hand**
 Temporary abutments titanium, crown and bridge						
 Esthomic® Abutments, incl. PS						
 Universal abutment, incl. PS Telescope abutment Gold-plastic abutment Logfit® Abutment		10.5 mm J4005.1601		10.5 mm J4005.2001		20 Ncm*
 Ceramic abutment						20 Ncm*
 Titanium bases CAD/CAM, crown incl. PS and bridge						
 Vario SR abutments, 20° and 30° angled						
 CAMLOG® CAM titanium blank, type IAC and ME						
<b>CAMLOG® Vario SR abutment screws</b>						
 Vario SR abutment, straight		11.9 mm J4007.1600		11.9 mm J4007.2000		20 Ncm*
<b>CAMLOG® Abutment screws with reduced head, light blue anodized</b>						
 COMFOUR® Bar abutments, 17° and 30° angled		9.5 mm J4004.1601		9.5 mm J4004.2001		20 Ncm*

\* with torque wrench J5320.1030

\*\* Optional for temporary abutments titanium: Torque after completed healing phase 20 Ncm.


All screws must be retightened with the corresponding torque after at least 5 minutes!

## Abutment-Prosthetic connection

Article	$\varnothing$ 3.3 mm	$\varnothing$ 3.8 mm	$\varnothing$ 4.3 mm	$\varnothing$ 5.0 mm	$\varnothing$ 6.0 mm
	M 1.6	M 2.0			
COMFOUR® Bar abutments, 17° and 30° angled		3.6 mm 		3.8 mm 	Tightening torque 15 Ncm*
	Vario SR prosthetic screw, yellow anodized				
Vario SR abutments, straight, 20° and 30° angled		4 mm 		J4005.2004	15 Ncm*

## Auxiliary screws Intra- and extraoral use

### Abutment-Prosthetic connection

Article	$\varnothing$ 3.3 mm	$\varnothing$ 3.8 mm	$\varnothing$ 4.3 mm	$\varnothing$ 5.0 mm	$\varnothing$ 6.0 mm
	M 1.6	M 2.0			
Scanning cap for bar abutments		3.6 mm 		3.8 mm 	Tightening torque tightened by hand
	Screws for bar abutments, for impression taking open tray and for soldering, light blue anodized				
COMFOUR® Bar abutments, straight, 17° and 30° angled	12 mm 		12.2 mm 	J4012.1610	J4012.2010
	17 mm 		17.2 mm 	J4012.1615	J4012.2015
	22 mm 		22.2 mm 	J4012.1620	J4012.2020
	Plastic screws for bar abutment, as fixation and bonding aid, beige				
	29 mm 		29.2 mm 	J4009.1627	J4009.2027

\* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

# Screw overview Lab screws – extraoral use

## Lab analog-Abutment connection

Article	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	Ø 6.0 mm	Tightening torque
	M 1.6			M 2.0		
Temporary abutments PEEK, incl. PS Scanbody ScanPost for Sirona® Scanbody						
Temporary abutments titanium, crown and bridge						
Esthomic® Abutments, incl. PS						
Universal abutment, incl. PS Telescope abutment Gold-plastic abutment			10.5 mm J4006.1601		10.5 mm J4006.2001	tightened by hand
Ceramic abutment						
Titanium bases CAD/CAM, crown incl. PS and bridge						
Vario SR abutments, 20° and 30° angled						
CAMLOG® CAM titanium blank, type IAC and ME						
<b>CAMLOG® Bonding aids**</b>						
Titanium bases CAD/CAM, crown and bridge		27.5 mm J4008.1600		27.5 mm J4008.2000		tightened by hand
<b>CAMLOG® Vario SR lab screws*, brown anodized</b>						
Vario SR abutment, straight		11.9 mm J4008.1600		11.9 mm J4008.2000		tightened by hand
<b>CAMLOG® Lab screws with reduced head*, light blue partially anodized</b>						
COMFOUR® Bar abutments, 17° and 30° angled		9.5 mm J4004.1600		9.5 mm J4004.2000		tightened by hand

\* Lab screws may not be used on patients.

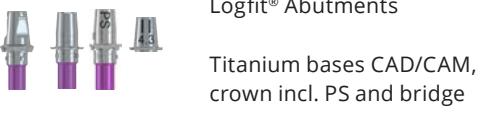
\*\* not available singly, are included in the packaging of the titanium base CAD/CAM.

## Abutment-Prosthetic connection

	$\varnothing$ 3.3 mm	$\varnothing$ 3.8 mm	$\varnothing$ 4.3 mm	$\varnothing$ 5.0 mm	$\varnothing$ 6.0 mm	
Article	Lab prosthetic screws for bar abutments*, brown anodized				Tightening torque	
Scanning cap for bar abutments						
COMFOUR® Bar abutment, straight, 17° and 30° angled		3.6 mm  J4013.1601		3.8 mm  J4013.2001		tightened by hand
Bar lab analog for bar abutments						
Vario SR prosthetic screw, yellow anodized						
Vario SR abutments, straight, 20° and 30° angled				4 mm  J4005.2004		tightened by hand
Vario SR analog						
Prosthetic screw for bar abutments*, for fabrication of the wax up on the bar sleeve for titanium bonding base, Passive-Fit, on the bar lab analog						
Titanium bonding base for bar abutments and bar sleeve for titanium bonding base, burn-out, Passive-Fit		5.5 mm  J4005.1602		5.5 mm  J4005.2002		tightened by hand

\* Lab screws may not be used on patients.

## Overview Tightening torque

Article	Instrument	Tightening torque
 Implant cover screw		
 Healing caps (incl. PS) cylindrical, wide body, bottleneck		
 Impression posts (incl. PS) Bite registration post		tightened by hand**
 Lab screws Lab screws with reduced head		
 Temporary abutments PEEK, incl. PS Temporary abutments titanium, crown and bridge	  	
 Abutment screws Abutment screws with reduced head	J5317.0510      J5317.0501      J5317.0502	
 Esthomic® Abutment, straight (incl. PS) Esthomic® Abutment, angled 15°/20° (incl. PS) Esthomic® Abutment, Inset	 	
 Universal abutment Telescope abutment Gold-plastic abutment Ceramic abutment		20 Ncm*
 Logfit® Abutments Titanium bases CAD/CAM, crown incl. PS and bridge		
 CAMLOG® CAM titanium blank, type IAC and ME		

\* with the torque wrench J5320.1030

\*\* Optional for temporary abutments titanium: torque after completed healing phase 20 Ncm.  
All screws must be retightened with the corresponding torque after at least 5 minutes!

Article	Instrument				Tightening torque
	3.3 mm	3.8 mm	4.3 mm	Ø 5.0 mm	
 Bar abutment, straight					20 Ncm*      30 Ncm*
 Bar abutment, 17° and 30° angled					20 Ncm*
 Scanning cap for bar abutments					tightened by hand
 Titanium cap for bar abutment, for crown/bridge					
 Crown base for bar abutment, burn-out	J5317.0510	J5317.0501	J5317.0502		15 Ncm*
 Bases for bar abutments burn-out, cast-on, solderable, laser-weldable					
 Titanium bonding bases for bar abutment, Passive-Fit					
 Locator R-Tx® Abutment	J5317.0504	J5317.0503		20 Ncm*	30 Ncm*
 Healing cap for bar abutment					
 Impression cap for bar abutment, closed tray (bridge/bar)					tightened by hand
 Ball abutments				20 Ncm*	30 Ncm*
 Locator® Abutments					
 Locator® Fixture for bar abutment					20 Ncm*
 Scanbodies					
 ScanPosts for Sirona® Scanbody					tightened by hand

\* with the torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

# Materials

Titanium Grade 4		
Properties (ASTM F67)		
Chemical structure (in %)	O	≤ 0.4
	Fe	≤ 0.5
	C	≤ 0.08
	N	≤ 0.05
	H	≤ 0.015
	Ti	Rest
Mechanical properties	Tensile strength	≥ 550 MPa
	Elongation at break	≥ 12 %

Titanium alloy Ti6Al4V ELI		
Properties (ASTM F136)		
Chemical structure (in %)	Al	5.5 – 6.5
	V	3.5 – 4.5
	Fe	≤ 0.25
	C	≤ 0.08
	N	≤ 0.05
	O	≤ 0.13
Mechanical properties	H	≤ 0.012
	Ti	Rest
Mechanical properties	Tensile strength	≥ 860 MPa
	Elongation at break	≥ 10 %

Cast-on gold alloy CAMLOG® Gold-plastic abutment		
Properties		
Chemical structure (in %)	Au	60
	Pd	20
	Pt	19
	Ir	1
Physical properties	Melting range	1400 – 1490 °C
	Density	17.5 g/cm³
	E-Modul	136 GPa
	Coefficient of thermal expansion (25 – 500°C)	11.9 µm/m· °C
	Coefficient of thermal expansion (25 – 600°C)	12.2 µm/m· °C
	Color	white
Mechanical properties		drawn
	Hardness HV5	> 215
	Tensile strength (Rm)	> 750 MPa
	0.2% Elongation limit (Rp 0.2%)	> 650 MPa
	Elongation at break	> 2 %

Cast-on gold alloy base for bar abutment		
Properties		
Chemical structure (in %)	Au	60
	Pt	19
	Pd	20
	Ir	1
Physical properties	Density	17.5 g/cm³
	Color	white
	Liquidus	1490 °C
	Solidus	1400 °C
	Coefficient of thermal expansion (25 – 500°C)	12.5 µm/m· °C
	Coefficient of thermal expansion (25 – 600°C)	12.6 µm/m· °C
Mechanical properties	E-Modul	136 GPa
		hardened 700 °C/30 min.
	Hardness HV5	210
	0.2 % Elongation limit	450 – 570 MPa
	Elongation at break	min. 10 %
	Tensile strength MPa	530 – 650

Solderable gold alloy base for bar abutment		
Properties		
Chemical structure (in %)	Au	68.60
	Pt	2.45
	Ag	11.85
	Pd	3.95
	Cu	10.60
	Zn	2.50
	Ir	0.05
	Rh	-
	Ru	-
Physical properties	Color	yellow
	Melting range	880 - 940 °C
Mechanical properties	Hardness annealed HV5	175
	hardened HV5	275
	self hardened HV5	240

# Index Alphabetical

## A

Abutment collets	84
Abutment screw, hex	79
Abutment screw, with reduced head, hex	72
Adapter for screw Implants	48
Adapter ISO shaft for angled hand piece	47
Aligning tool	70
ALTApin applicator	54
ALTApin magazine	56
ALTApin membrane fixator	55
ALTApin pricker	55
ALTApin pricker, insert	56
ALTApin set	54
ALTApin single patient drill, ISO shaft	55
ALTApin surgery mallet	55
ALTApin tray	54
Appointment pad	91

## B

Ball abutment analogs	74
Ball abutments, male part	73
Bar abutment	69
Bar Implant analog for bar abutments	70
Bar lab analog for bar abutments	70
Bar sleeve for titanium bonding base	71
Baring drill for cover screw	44
Base for bar abutment	71
Base for bar abutment, titanium	71
Bite registration caps	61
Bite registration posts	61
Bone profiler	44

## C

CAM Titanium blank	66
Cardanic driver	47
Cleaning cannula	49
Cleaning needle	49
Collet for CAM blank, type IAC	66
COMFOUR® Patient brochure	90
Countersink	44
Crown base for bar abutment	71
CT-tube	17

## D

Demonstration model, acrylic glass	89
Dense bone drill PROGRESSIVE-LINE	23
Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE	23, 39
Depth stop SCREW-LINE	44
DIM-Analog® for the CAMLOG® Implant System	61
Drill extension ISO shaft for instruments with internal irrigation not for drills with internal irrigation	42 45
Drill for CT-tube	17
Drill PROGRESSIVE-LINE Flex	27
Driver for ball abutment	80
Driver for impression cap and healing cap for bar abutments	70, 81
Driver for Locator®	81
Driver for screw Implants	46
Driver for straight bar abutment	80, 81

## E

Edentulous mandible	89
Esthomic® Abutments	62, 63

## E

Esthomic® Abutments PS	63
Esthomic® Abutments, Inset	63
Esthomic® Selection abutments	85

## F

Form drill PROGRESSIVE-LINE	23
Form drill SCREW-LINE	39
Form drill SCREW-LINE Cortical bone	39

## G

Gingiva height indicator, straight	70
Gold-plastic abutment	67
Guide System check-up pin	42
Guide System check-up pin PROGRESSIVE-LINE	32
Guide System dense bone drill PROGRESSIVE-LINE	31
Guide System form drill PROGRESSIVE-LINE	31
Guide System form drill for Ø 3.8 mm under preparation PROGRESSIVE-LINE	31
Guide System form drill SCREW-LINE, Cortical bone	41
Guide System gingiva punch	41
Guide System gingiva punch PROGRESSIVE-LINE	30
Guide System guiding sleeve	41
Guide System guiding sleeve PROGRESSIVE-LINE	32
Guide System Insertion post, screw-mounted	32, 42
Guide System pilot drill PROGRESSIVE-LINE	30
Guide System pilot drill set	40
Guide System pre-drill PROGRESSIVE-LINE	31
Guide System seating tool	42
Guide System setting tool PROGRESSIVE-LINE	32
Guide System surgery set, SCREW-LINE	40

## G

Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30
Guide System template drill	42
Guide System template drill PROGRESSIVE-LINE	32
Guiding pin for bone profiler	44

## H

Handle for CAMLOG®/CONELOG® Implant analog	83
Healing cap for bar abutment	70
Healing cap	57
Healing cap PS	58
Holding key for insertion post	48
Holding sleeve for screw Implants	48

## I

Implant analog	61
Implant cover screw	57
Implant pass	90
Impression cap for bar abutment, closed tray	70
Impression caps for impression post, closed tray	60
Impression posts	60
Impression posts PS	60

## L

Lab analog	61
Lab prosthetic screw for bar abutment, hex	72
Lab screw, hex	79
Lab screw, with reduced head, hex	72
Lamella retention insert	74
Locator® Abutment	76
Locator® Abutment holder sleeve	81

# Index Alphabetical

## L

Locator® Analog	76
Locator® Angle measurement guide	81
Locator® Block out spacer	77
Locator® Fixture for bar abutment	72
Locator® Impression cap	76
Locator® Instrument	81
Locator® Male processing package	77
Locator® Male processing package for extended range	77
Locator® Parallel post	81
Locator® Processing replacement male	77
Locator® Replacement male	77, 78
Locator® Replacement male for extended range	78
Locator R-Tx® Abutment	74
Locator R-Tx® Analog	74, 75
Locator R-Tx® Impression coping	74
Locator R-Tx® Retention insert	75, 76
Locator R-Tx® Retention insert tool	82
Locator R-Tx® Processing insert	75
Locator R-Tx® Processing spacer	75
Locator R-Tx® Titanium housing	75
Logfit® Abutments	68
Logfit® Analog	68
Logfit® Impression caps	68
Logfit® Plastic copings	68

## M

Manual screwdriver, hex	49, 83
Matrix CM Dalbo®-Plus	73

## M

Modeling aids for CAMLOG® Titanium bases CAD/CAM	65
O	
Orientation gauge for COMFOUR®	70
Osteotome SCREW-LINE	50, 51, 52, 53
Osteotomy set CAMLOG®/CONELOG® SCREW-LINE	50, 51, 52, 53
P	
Paralleling pin PROGRESSIVE-LINE	23
Paralleling pin SCREW-LINE	45
Patient advice sheets	90
Patient brochure	90
Pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	22
CAMLOG®/CONELOG® SCREW-LINE	38
PickUp instrument	47
Pilot drill	43
Pilot drill SCREW-LINE	43
Plastic screw for bar abutment	73
Point drill	43
Polishing protection for caps and bases for bar abutment	72
Poster	91
Pre-drill SCREW-LINE	43
Pre-Osteotome SCREW-LINE	50, 51, 52, 53
Presentation folder	90
Profile drill PROGRESSIVE-LINE Flex	27
PROGRESSIVE-LINE Implant for practice	88
PROGRESSIVE-LINE Implant, Promote® plus	19
PROGRESSIVE-LINE Macro model	89
Prosthetic screw for bar abutments	72

## P

Prosthetic set	82
Prosthetic tray	82
Prosthetic tray universal	82

## R

Ramers for dilating the plaster model, for universal holder	84
Removal adapter for CAMLOG® and CONELOG®	23
Reworking reamer, for base for bar abutment	84
Round bur	43

## S

Scanbodies	65
Scanning cap for bar abutments	70
ScanPosts for Sirona® Scanbody	65
Screw, hex	72, 73
Screwdriver Activator	80
Screwdriver, hex	48, 49, 82, 83
SCREW-LINE Implant for practice	88
SCREW-LINE Implant, Promote®	34, 35
SCREW-LINE Implant, Promote® plus	34, 35
SCREW-LINE Macro model	89
Selection abutment kit	85

## Surgery set

CAMLOG®/CONELOG® PROGRESSIVE-LINE	22
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	26
CAMLOG®/CONELOG® SCREW-LINE	38
Surgery tray	
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	26
CAMLOG®/CONELOG® SCREW-LINE	38

## Surgery wash tray

CAMLOG®/CONELOG® PROGRESSIVE-LINE	22
CAMLOG®/CONELOG® SCREW-LINE	38

## T

Tap adapter	45
Tap PROGRESSIVE-LINE	23
Tap SCREW-LINE	39
Telescope abutments, for double crown restorations	79
Temporary abutment, titanium alloy	62
Temporary abutments, PEEK	62
Temporary abutments PS, PEEK, for Platform Switching	62
Titanium bases CAD/CAM	64
Titanium bases CAD/CAM PS	64
Titanium bonding base for bar abutment	71
Titanium cap for bar abutment	70, 71
Titanium cap without retention for bar abutment, for bridge	71
Torque wrench	80

## U

Universal abutments	67, 79
Universal abutments PS	67, 79
Universal holder	84

## W

Wrench adapter	27
----------------	----

## X

X-Ray Planning foil 1.25:1	
CAMLOG® PROGRESSIVE-LINE Implants	16
CAMLOG® SCREW-LINE Implants	16
X-Ray Planning foil 1.4:1	
CAMLOG® PROGRESSIVE-LINE Implants	16
CAMLOG® SCREW-LINE Implants	16
X-Ray Transfer pictures 1.25:1	
CAMLOG® SCREW-LINE Implants	16

# Index Article number

05003503	Matrix CM Dalbo®-Plus	73	A2222.2200	CT-tube	17
05003504	Lamella retention insert	74	B1012	Point drill	43
07000389	Screwdriver Activator	80		Healing cap, bottleneck	
			J2011.3340	Ø 3.3 mm, GH 4.0 mm	57
08394	Locator® Abutment holder sleeve	81	J2011.3840	Ø 3.8 mm, GH 4.0 mm	57
	Locator R-Tx® Retention insert		J2011.3860	Ø 3.8 mm, GH 6.0 mm	57
30001-01	Ø 3.3/3.8/4.3/5.0 mm, gray	75	J2011.4340	Ø 4.3 mm, GH 4.0 mm	57
30002-01	Ø 3.3/3.8/4.3/5.0 mm, blue	75	J2011.4360	Ø 4.3 mm, GH 6.0 mm	57
30003-01	Ø 3.3/3.8/4.3/5.0 mm, pink	76	J2011.5040	Ø 5.0 mm, GH 4.0 mm	57
30004-01	Ø 3.3/3.8/4.3/5.0 mm, white	76	J2011.5060	Ø 5.0 mm, GH 6.0 mm	57
			J2011.6040	Ø 6.0 mm, GH 4.0 mm	57
			J2011.6060	Ø 6.0 mm, GH 6.0 mm	57
	Locator R-Tx® Processing insert				
30012-01	Ø 3.3/3.8/4.3/5.0 mm	75		Healing cap, wide body	
			J2014.3320	Ø 3.3 mm, GH 2.0 mm	57
	Locator R-Tx® Titanium housing		J2014.3340	Ø 3.3 mm, GH 4.0 mm	57
30013-01	Ø 3.3/3.8/4.3/5.0 mm	75	J2014.3820	Ø 3.8 mm, GH 2.0 mm	57
			J2014.3840	Ø 3.8 mm, GH 4.0 mm	57
	Locator R-Tx® Analog		J2014.3860	Ø 3.8 mm, GH 6.0 mm	57
30014-01	Ø 3.3 mm	74	J2014.4320	Ø 4.3 mm, GH 2.0 mm	57
30015-01	Ø 3.8/4.3 mm	75	J2014.4340	Ø 4.3 mm, GH 4.0 mm	57
30016-01	Ø 5.0 mm	75	J2014.4360	Ø 4.3 mm, GH 6.0 mm	57
			J2014.5020	Ø 5.0 mm, GH 2.0 mm	57
	Locator R-Tx® Impression coping		J2014.5040	Ø 5.0 mm, GH 4.0 mm	57
30017-01	Ø 3.3/3.8/4.3/5.0 mm	74	J2014.5060	Ø 5.0 mm, GH 6.0 mm	57
			J2014.6020	Ø 6.0 mm, GH 2.0 mm	57
	Locator R-Tx® Processing spacer		J2014.6040	Ø 6.0 mm, GH 4.0 mm	57
30018-01	Ø 3.3/3.8/4.3/5.0 mm	75	J2014.6060	Ø 6.0 mm, GH 6.0 mm	57
30021-01	Locator R-Tx® Retention insert tool	82		Healing cap, cylindrical	
			J2015.3320	Ø 3.3 mm, GH 2.0 mm	57
	Locator R-Tx® Abutment		J2015.3340	Ø 3.3 mm, GH 4.0 mm	57
30800-01	Ø 3.3 mm, GH 1.0 mm	74	J2015.3820	Ø 3.8 mm, GH 2.0 mm	57
30800-02	Ø 3.3 mm, GH 2.0 mm	74	J2015.3840	Ø 3.8 mm, GH 4.0 mm	57
30800-03	Ø 3.3 mm, GH 3.0 mm	74	J2015.3860	Ø 3.8 mm, GH 6.0 mm	57
30800-04	Ø 3.3 mm, GH 4.0 mm	74	J2015.4320	Ø 4.3 mm, GH 2.0 mm	57
30801-01	Ø 3.8 mm, GH 1.0 mm	74	J2015.4340	Ø 4.3 mm, GH 4.0 mm	57
30801-02	Ø 3.8 mm, GH 2.0 mm	74	J2015.4360	Ø 4.3 mm, GH 6.0 mm	57
30801-03	Ø 3.8 mm, GH 3.0 mm	74	J2015.5020	Ø 5.0 mm, GH 2.0 mm	57
30801-04	Ø 3.8 mm, GH 4.0 mm	74	J2015.5040	Ø 5.0 mm, GH 4.0 mm	57
30801-05	Ø 3.8 mm, GH 5.0 mm	74	J2015.5060	Ø 5.0 mm, GH 6.0 mm	57
30802-01	Ø 4.3 mm, GH 1.0 mm	74	J2015.6020	Ø 6.0 mm, GH 2.0 mm	57
30802-02	Ø 4.3 mm, GH 2.0 mm	74	J2015.6040	Ø 6.0 mm, GH 4.0 mm	57
30802-03	Ø 4.3 mm, GH 3.0 mm	74	J2015.6060	Ø 6.0 mm, GH 6.0 mm	57
30802-04	Ø 4.3 mm, GH 4.0 mm	74			
30802-05	Ø 4.3 mm, GH 5.0 mm	74		Implant cover screw	
30803-01	Ø 5.0 mm, GH 1.0 mm	74	J2019.3300	Ø 3.3 mm	57
30803-02	Ø 5.0 mm, GH 2.0 mm	74	J2019.3800	Ø 3.8 mm	57
30803-03	Ø 5.0 mm, GH 3.0 mm	74	J2019.4300	Ø 4.3 mm	57
30803-04	Ø 5.0 mm, GH 4.0 mm	74	J2019.5000	Ø 5.0 mm	57
30803-05	Ø 5.0 mm, GH 5.0 mm	74	J2019.6000	Ø 6.0 mm	57
A2002.2000	CT-tube	17		Healing cap for bar abutment	
			J2029.4300	Ø 3.3/3.8/4.3 mm	70
	Drill for CT-tube		J2029.6000	Ø 5.0 mm	70
A2050.2600	Ø 2.6 mm	17			
A2050.2800	Ø 2.8 mm	17			

	Impression caps for impression post, closed tray	J2253.0112	Locator® Male processing package for extended range	77
J2111.3300	Ø 3.3 mm	60		
J2111.3800	Ø 3.8 mm	60	J2253.0200	Locator® Impression cap
J2111.4300	Ø 4.3 mm	60		
J2111.5000	Ø 5.0 mm	60		Locator® Analog
J2111.6000	Ø 6.0 mm	60	J2253.0340	Ø 3.3/3.8/4.3 mm
			J2253.0350	Ø 5.0 mm
	Bite registration caps			
J2112.3300	Ø 3.3 mm	61	J2253.0401	Locator® Block out spacer
J2112.3800	Ø 3.8 mm	61		
J2112.4300	Ø 4.3 mm	61	J2253.0402	Locator® Processing replacement male
J2112.5000	Ø 5.0 mm	61		
J2112.6000	Ø 6.0 mm	61		Locator® Replacement male
	Impression cap, for bar abutment, closed tray (bridge/bar)		J2253.1002	Ø 3.3/3.8/4.3/5.0 mm, blue
J2129.4300	Ø 3.3/3.8/4.3 mm, short	70	J2253.1003	Ø 3.3/3.8/4.3/5.0 mm, pink
J2129.4310	Ø 3.3/3.8/4.3 mm, long	70	J2253.1005	Ø 3.3/3.8/4.3/5.0 mm, clear
J2129.6000	Ø 5.0 mm, short	70		
J2129.6010	Ø 5.0 mm, long	70	J2253.2000	Ø 3.8/4.3/5.0 mm, gray
	Bite registration posts		J2253.2002	Ø 3.8/4.3/5.0 mm, red
J2140.3300	Ø 3.3 mm	61	J2253.2003	Ø 3.8/4.3/5.0 mm, orange
J2140.3800	Ø 3.8 mm	61	J2253.2004	Ø 3.8/4.3/5.0 mm, green
J2140.4300	Ø 4.3 mm	61		Locator® Abutment
J2140.5000	Ø 5.0 mm	61	J2253.3310	Ø 3.3 mm, GH 1.0 mm
J2140.6000	Ø 6.0 mm	61	J2253.3320	Ø 3.3 mm, GH 2.0 mm
	Modeling aids for CAMLOG®		J2253.3330	Ø 3.3 mm, GH 3.0 mm
	Titanium bases CAD/CAM		J2253.3340	Ø 3.3 mm, GH 4.0 mm
J2244.3302	Ø 3.3 mm	65	J2253.3810	Ø 3.8 mm, GH 1.0 mm
J2244.3802	Ø 3.8 mm	65	J2253.3820	Ø 3.8 mm, GH 2.0 mm
J2244.4302	Ø 4.3 mm	65	J2253.3830	Ø 3.8 mm, GH 3.0 mm
J2244.5002	Ø 5.0 mm	65	J2253.3840	Ø 3.8 mm, GH 4.0 mm
J2244.6002	Ø 6.0 mm	65	J2253.3850	Ø 3.8 mm, GH 5.0 mm
	Ball abutments, male part		J2253.4310	Ø 4.3 mm, GH 1.0 mm
J2249.3315	Ø 3.3 mm, GH 1.5 mm	73	J2253.4320	Ø 4.3 mm, GH 2.0 mm
J2249.3330	Ø 3.3 mm, GH 3.0 mm	73	J2253.4330	Ø 4.3 mm, GH 3.0 mm
J2249.3815	Ø 3.8 mm, GH 1.5 mm	73	J2253.4340	Ø 4.3 mm, GH 4.0 mm
J2249.3830	Ø 3.8 mm, GH 3.0 mm	73	J2253.4350	Ø 4.3 mm, GH 5.0 mm
J2249.3845	Ø 3.8 mm, GH 4.5 mm	73	J2253.5010	Ø 5.0 mm, GH 1.0 mm
J2249.4315	Ø 4.3 mm, GH 1.5 mm	73	J2253.5020	Ø 5.0 mm, GH 2.0 mm
J2249.4330	Ø 4.3 mm, GH 3.0 mm	73	J2253.5030	Ø 5.0 mm, GH 3.0 mm
J2249.4345	Ø 4.3 mm, GH 4.5 mm	73	J2253.5040	Ø 5.0 mm, GH 4.0 mm
J2249.5015	Ø 5.0 mm, GH 1.5 mm	73	J2253.5050	Ø 5.0 mm, GH 5.0 mm
	Locator® Fixture for bar abutment			
J2249.5030	Ø 5.0 mm, GH 3.0 mm	73	J2253.4301	Ø 3.3/3.8/4.3 mm
J2249.5045	Ø 5.0 mm, GH 4.5 mm	73	J2253.6001	Ø 5.0 mm
	Driver for Locator®	81		Bar abutment, straight
J2253.0002	Locator® Instrument	81	J2254.3305	Ø 3.3 mm, GH 0.5 mm
J2253.0003	Locator® Angle measurement guide	81	J2254.3320	Ø 3.3 mm, GH 2.0 mm
J2253.0004	Locator® Parallel post	81	J2254.3805	Ø 3.8 mm, GH 0.5 mm
J2253.0102	Locator® Male processing package	77	J2254.3820	Ø 3.8 mm, GH 2.0 mm
			J2254.3840	Ø 3.8 mm, GH 4.0 mm
			J2254.4305	Ø 4.3 mm, GH 0.5 mm
			J2254.4320	Ø 4.3 mm, GH 2.0 mm
			J2254.4340	Ø 4.3 mm, GH 4.0 mm
			J2254.5005	Ø 5.0 mm, GH 0.5 mm

# Index Article number

	Bar abutment, straight		Logfit® Impression caps		
J2254.5020	Ø 5.0 mm, GH 2.0 mm	69	J2551.4300	Ø 3.8/4.3 mm	
J2254.5040	Ø 5.0 mm, GH 4.0 mm	69	J2551.6000	Ø 5.0/6.0 mm	
	Crown base for bar abutment		Logfit® Analog		
J2256.4306	Ø 3.3/3.8/4.3 mm	71	J2552.4300	Ø 3.8/4.3 mm	
J2256.6006	Ø 5.0 mm	71	J2552.6000	Ø 5.0/6.0 mm	
	Base for bar abutment, burn-out		Logfit® Plastic copings		
J2257.4301	Ø 3.3/3.8/4.3 mm	71	J2553.4301	Ø 3.8/4.3 mm, for bridges	
J2257.6001	Ø 5.0 mm	71	J2553.4302	Ø 3.8/4.3 mm, for crowns	
	Base for bar abutment, solderable		J2553.6001	Ø 5.0/6.0 mm, for bridges	
J2258.4300	Ø 3.3/3.8/4.3 mm	71	J2553.6002	Ø 5.0/6.0 mm, for crowns	
J2258.6000	Ø 5.0 mm	71		Scanning cap for bar abutments	
	Titanium cap for bar abutment		J2610.4300	Ø 3.3/3.8/4.3 mm	
J2259.4301	Ø 3.3/3.8/4.3 mm, for crown	70	J2610.6000	Ø 5.0 mm	
J2259.4302	Ø 3.3/3.8/4.3 mm, for bridge	71		Ball abutment analogs	
J2259.6001	Ø 5.0 mm, for crown	70	J3015.3300	Ø 3.3 mm	
J2259.6002	Ø 5.0 mm, for bridge	71	J3015.3800	Ø 3.8 mm	
	Titanium cap without retention for bar abutment, for bridge		J3015.4300	Ø 4.3 mm	
J2259.4322	Ø 3.3/3.8/4.3 mm	71	J3015.5000	Ø 5.0 mm	
J2259.6022	Ø 5.0 mm	71		Bar lab analog for bar abutments	
	Titanium bonding base for bar abutment		J3020.4300	Ø 3.3/3.8/4.3 mm	
J2260.4301	Ø 3.3/3.8/4.3 mm	71	J3020.6000	Ø 5.0 mm	
J2260.6001	Ø 5.0 mm	71		Polishing protection for caps and bases for bar abutment	
	Bar sleeve for titanium bonding base		J3021.4300	Ø 3.3/3.8/4.3 mm	
J2261.4301	Ø 3.3/3.8/4.3 mm	71	J3021.6000	Ø 5.0 mm	
J2261.6001	Ø 5.0 mm	71		Handle for CAMLOG®/CONELOG® Implant analog	
	Base for bar abutment,		J3025.0010	Ø 3.3/3.8/4.3 mm	
J2262.4300	Ø 3.3/3.8/4.3 mm, laser-weldable	71	J3025.0015	Ø 5.0/6.0 mm	
J2262.6000	Ø 5.0 mm, laser-weldable	71		Bar Implant analog for bar abutments	
J2263.4300	Ø 3.3/3.8/4.3 mm, cast-on	71	J3025.4300	Ø 3.3/3.8/4.3 mm	
J2263.6000	Ø 5.0 mm, cast-on	71	J3025.6000	Ø 5.0 mm	
J2269.0003	Aligning tool 17°	70		Gingiva height indicator, straight	
J2269.0004	Aligning tool 30°	70		J3550.3300	Ø 3.3 mm
J2269.0005	Aligning tool 17°	70		J3550.3800	Ø 3.8 mm
J2269.0006	Aligning tool 30°	70		J3550.4300	Ø 4.3 mm
	Temporary abutment, bridge, titanium alloy		J3550.5000	Ø 5.0 mm	
J2339.3300	Ø 3.3 mm	62	J3551.0001	Orientation gauge for COMFOUR®	
J2339.3800	Ø 3.8 mm	62		Ramars for dilating the plaster model, for universal holder	
J2339.4300	Ø 4.3 mm	62	J3706.3300	Ø 3.3 mm	
J2339.5000	Ø 5.0 mm	62	J3706.3800	Ø 3.8 mm	
J2339.6000	Ø 6.0 mm	62	J3706.4300	Ø 4.3 mm	
	Titanium bases CAD/CAM, bridge		J3706.5000	Ø 5.0 mm	
J2344.3348	Ø 3.3 mm	64	J3706.6000	Ø 6.0 mm	
J2344.3848	Ø 3.8 mm	64		Universal holder, incl. Lab screws and Abutment collet	
J2344.4348	Ø 4.3 mm	64			
J2344.5048	Ø 5.0 mm	64			
J2344.6048	Ø 6.0 mm	64			

J3709.0015	Universal holder	84		Abutment screw, hex Ø 5.0/6.0 mm, M 2.0	79
	Abutment collets		J4005.2001		
J3709.3300	Ø 3.3 mm	84		Lab screw, hex	79
J3709.3800	Ø 3.8 mm	84	J4006.1601	Ø 3.3/3.8/4.3 mm, M 1.6	79
J3709.4300	Ø 4.3 mm	84	J4006.2001	Ø 5.0/6.0 mm, M 2.0	79
J3709.5000	Ø 5.0 mm	84			
J3709.6000	Ø 6.0 mm	84		Plastic screw for bar abutment M 1.6 M 2.0	73
	Reworking reamer, for base for bar abutment		J4009.1627		73
	plane surface/cone seat		J4009.2027		73
J3711.0010	Ø 3.3/3.8/4.3 mm	84	J4012.1601	Prosthetic screw for bar abutments Ø 3.3/3.8/4.3 mm	72
J3711.0015	Ø 5.0/6.0 mm	84	J4012.2001	Ø 5.0 mm	72
	screw seat		J4012.1610	Screw, hex	72
J3711.0020	Ø 3.3/3.8/4.3 mm	84	J4012.1615	L 10 mm, M 1.6	72
J3711.0025	Ø 5.0/6.0 mm	84	J4012.1620	L 15 mm, M 1.6	72
	Guide System Seating tool		J4012.2010	L 20 mm, M 1.6	73
J3716.3300	Ø 3.3 mm	42	J4012.2015	L 10 mm, M 2.0	72
J3716.4300	Ø 3.8/4.3 mm	42	J4012.2020	L 15 mm, M 2.0	72
	Guide System setting tool		J4012.2020	L 20 mm, M 2.0	73
	PROGRESSIVE-LINE			Lab prosthetic screw for bar abutment Ø 3.3/3.8/4.3 mm	72
J3717.3300	Ø 3.3 mm	32	J4013.2001	Ø 5.0 mm	72
J3717.4300	Ø 3.8/4.3 mm	32			
J3717.5000	Ø 5.0 mm	32		Drill extension ISO shaft	
	Guide System Template drill		J5002.0005	for instruments with internal irrigation	42
J3733.3300	Ø 3.3 mm	42	J5002.0006	not for instruments with internal	45
J3733.4300	Ø 3.8/4.3 mm	42		irrigation	
	Guide System Guiding sleeve		J5002.0011	Adapter ISO shaft	47
J3734.3303	Ø 3.3 mm	41	J5002.0012	Cleaning needle	49
J3734.3803	Ø 3.8 mm	41	J5002.0013	Wrench adapter	27
J3734.4303	Ø 4.3 mm	41	J5002.0020	Cleaning cannula	49
	Guide System template drill				
	PROGRESSIVE-LINE				
J3753.3300	Ø 3.3 mm	32	J5002.3300	Guiding pin for bone profiler Ø 3.3 mm	44
J3753.4300	Ø 3.8/4.3 mm	32	J5002.3800	Ø 3.8 mm	44
J3753.5000	Ø 5.0 mm	32	J5002.4300	Ø 4.3 mm	44
	Guide System guiding sleeve		J5002.5000	Ø 5.0 mm	44
	PROGRESSIVE-LINE				
J3754.3301	Ø 3.3 mm	32			
J3754.3801	Ø 3.8 mm	32		Bone profiler	
J3754.4301	Ø 4.3 mm	32	J5003.3350	Ø 3.3 mm, Ø 5.0 mm	44
J3754.5001	Ø 5.0 mm	32	J5003.4360	Ø 3.8/4.3 mm, Ø 6.0 mm	44
	Lab screw with reduced head, hex		J5003.5070	Ø 5.0 mm, Ø 7.0 mm	44
J4004.1600	Ø 3.3/3.8/4.3 mm, M 1.6	72			
J4004.2000	Ø 5.0 mm, M 2.0	72	J5004.3300	Baring drill for cover screw Ø 3.3 mm	44
	Abutment screw with reduced head, hex		J5004.3800	Ø 3.8 mm	44
J4004.1601	Ø 3.3/3.8/4.3 mm, M 1.6	72	J5004.4300	Ø 4.3 mm	44
J4004.2001	Ø 5.0 mm, M 2.0	72	J5004.5000	Ø 5.0 mm	44
	Abutment screw, hex			Countersink	
J4005.1601	Ø 3.3/3.8/4.3 mm, M 1.6	79	J5006.3346	Ø 3.3 mm, Ø 4.6 mm	44
			J5006.3852	Ø 3.8 mm, Ø 5.2 mm	44

# Index Article number

	Countersink			Form drill SCREW-LINE	
J5006.4356	Ø 4.3 mm, Ø 5.6 mm	44	J5062.4313	Ø 4.3 mm, L 13 mm	39
J5006.5063	Ø 5.0 mm, Ø 6.3 mm	44	J5062.4316	Ø 4.3 mm, L 16 mm	39
			J5062.5009	Ø 5.0 mm, L 9 mm	39
	Depth stop SCREW-LINE for pilot drill and pre-drill		J5062.5011	Ø 5.0 mm, L 11 mm	39
J5015.0009	L 9 mm	44	J5062.5013	Ø 5.0 mm, L 13 mm	39
J5015.0011	L 11 mm	44	J5062.6009	Ø 6.0 mm, L 9 mm	39
J5015.0013	L 13 mm	44	J5062.6011	Ø 6.0 mm, L 11 mm	39
			J5062.6013	Ø 6.0 mm, L 13 mm	39
	Depth stop for form drills		J5062.6016	Ø 6.0 mm, L 16 mm	39
	PROGRESSIVE-LINE and SCREW-LINE				
J5015.3300	Ø 3.3 mm	23, 39		Guide System Pilot drill set	
J5015.3800	Ø 3.8 mm	23, 39	J5063.3311	Ø 3.3 mm, L 5/9/11 mm	40
J5015.4300	Ø 4.3 mm	23, 39	J5063.3313	Ø 3.3 mm, L 5/9/11/13 mm	40
J5015.5000	Ø 5.0 mm	23, 39	J5063.4309	Ø 3.8/4.3 mm, L 5/9 mm	40
J5015.6000	Ø 6.0 mm	39	J5063.4311	Ø 3.8/4.3 mm, L 5/9/11 mm	40
			J5063.4313	Ø 3.8/4.3 mm, L 5/9/11/13 mm	40
	Guide System Gingiva punch		J5064.3316	Ø 3.3 mm, L 16 mm	40
J5041.3303	Ø 3.3 mm, SCREW-LINE	41	J5064.4316	Ø 3.8/4.3 mm, L 16 mm	40
J5041.3304	Ø 3.3 mm, PROGRESSIVE-LINE	30		Guide System Surgery set, SCREW-LINE	
J5041.3803	Ø 3.8 mm, SCREW-LINE	41	J5065.3311	Ø 3.3 mm, L 5/9/11 mm	40
J5041.3804	Ø 3.8 mm, PROGRESSIVE-LINE	30	J5065.3313	Ø 3.3 mm, L 5/9/11/13 mm	40
J5041.4303	Ø 4.3 mm, SCREW-LINE	41	J5065.3809	Ø 3.8 mm, L 5/9 mm	40
J5041.4304	Ø 4.3 mm, PROGRESSIVE-LINE	30	J5065.3811	Ø 3.8 mm, L 5/9/11 mm	40
J5041.5004	Ø 5.0 mm, PROGRESSIVE-LINE	30	J5065.3813	Ø 3.8 mm, L 5/9/11/13 mm	40
J5050.2300	Round bur	43	J5065.4309	Ø 4.3 mm, L 5/9 mm	40
			J5065.4311	Ø 4.3 mm, L 5/9/11 mm	40
J5051.2000	Pilot drill SCREW-LINE	43	J5065.4313	Ø 4.3 mm, L 5/9/11/13 mm	40
			J5066.3316	Ø 3.3 mm, L 16 mm	40
J5051.2003	Pilot drill	43	J5066.3816	Ø 3.8 mm, L 16 mm	40
			J5066.4316	Ø 4.3 mm, L 16 mm	40
J5051.2800	Pre-drill SCREW-LINE	43		Guide System Form drill, SCREW-LINE, Cortical Bone	
	Form drill SCREW-LINE Cortical bone		J5068.3311	Ø 3.3 mm, L 11 mm	41
J5053.3316	Ø 3.3 mm	39	J5068.3313	Ø 3.3 mm, L 13 mm	41
J5053.3816	Ø 3.8 mm	39	J5068.3316	Ø 3.3 mm, L 16 mm	41
J5053.4316	Ø 4.3 mm	39	J5068.3809	Ø 3.8 mm, L 9 mm	41
J5053.5016	Ø 5.0 mm	39	J5068.3811	Ø 3.8 mm, L 11 mm	41
J5053.6016	Ø 6.0 mm	39	J5068.3813	Ø 3.8 mm, L 13 mm	41
	Tap SCREW-LINE		J5068.3816	Ø 3.8 mm, L 16 mm	41
J5054.3309	Ø 3.3 mm	39	J5068.4309	Ø 4.3 mm, L 9 mm	41
J5054.3809	Ø 3.8 mm	39	J5068.4311	Ø 4.3 mm, L 11 mm	41
J5054.4309	Ø 4.3 mm	39	J5068.4313	Ø 4.3 mm, L 13 mm	41
J5054.5009	Ø 5.0 mm	39	J5068.4316	Ø 4.3 mm, L 16 mm	41
J5054.6009	Ø 6.0 mm	39		Form drill PROGRESSIVE-LINE	
	Form drill SCREW-LINE		J5070.3309	Ø 3.3 mm, L 9 mm	23
J5062.3309	Ø 3.3 mm, L 9 mm	39	J5070.3311	Ø 3.3 mm, L 11 mm	23
J5062.3311	Ø 3.3 mm, L 11 mm	39	J5070.3313	Ø 3.3 mm, L 13 mm	23
J5062.3313	Ø 3.3 mm, L 13 mm	39	J5070.3316	Ø 3.3 mm, L 16 mm	23
J5062.3316	Ø 3.3 mm, L 16 mm	39	J5070.3809	Ø 3.8 mm, L 9 mm	23
J5062.3809	Ø 3.8 mm, L 9 mm	39	J5070.3811	Ø 3.8 mm, L 11 mm	23
J5062.3811	Ø 3.8 mm, L 11 mm	39	J5070.3813	Ø 3.8 mm, L 13 mm	23
J5062.3813	Ø 3.8 mm, L 13 mm	39	J5070.3816	Ø 3.8 mm, L 16 mm	23
J5062.3816	Ø 3.8 mm, L 16 mm	39	J5070.4309	Ø 4.3 mm, L 9 mm	23
J5062.4309	Ø 4.3 mm, L 9 mm	39	J5070.4311	Ø 4.3 mm, L 11 mm	23
J5062.4311	Ø 4.3 mm, L 11 mm	39	J5070.4313	Ø 4.3 mm, L 13 mm	23

	<b>Form drill PROGRESSIVE-LINE</b>		<b>Guide System form drill</b>
J5070.4316	Ø 4.3 mm, L 16 mm	23	PROGRESSIVE-LINE
J5070.5009	Ø 5.0 mm, L 9 mm	23	Ø 5.0 mm, L 13 mm
J5070.5011	Ø 5.0 mm, L 11 mm	23	Ø 5.0 mm, L 16 mm
J5070.5013	Ø 5.0 mm, L 13 mm	23	
J5070.5016	Ø 5.0 mm, L 16 mm	23	<b>Guide System form drill for Ø 3.8 mm under preparation PROGRESSIVE-LINE</b>
	<b>Tap PROGRESSIVE-LINE</b>		J5077.3309 Ø 3.3 mm, L 9 mm
J5071.3300	Ø 3.3 mm	23	J5077.3311 Ø 3.3 mm, L 11 mm
J5071.3800	Ø 3.8 mm	23	J5077.3313 Ø 3.3 mm, L 13 mm
J5071.4300	Ø 4.3 mm	23	J5077.3316 Ø 3.3 mm, L 16 mm
J5071.5000	Ø 5.0 mm	23	
	<b>Dense bone drill PROGRESSIVE-LINE</b>		<b>Guide System dense bone drill</b>
J5072.3300	Ø 3.3 mm	23	PROGRESSIVE-LINE
J5072.3800	Ø 3.8 mm	23	J5078.3311 Ø 3.3 mm, L 11 mm
J5072.4300	Ø 4.3 mm	23	J5078.3313 Ø 3.3 mm, L 13 mm
J5072.5000	Ø 5.0 mm	23	J5078.3316 Ø 3.3 mm, L 16 mm
	<b>Guide System pilot drill</b>		J5078.3809 Ø 3.8 mm, L 9 mm
	<b>PROGRESSIVE-LINE</b>		J5078.3811 Ø 3.8 mm, L 11 mm
J5074.3305	Ø 3.3 mm, L 5 mm	30	J5078.3813 Ø 3.8 mm, L 13 mm
J5074.3309	Ø 3.3 mm, L 9 mm	30	J5078.3816 Ø 3.8 mm, L 16 mm
J5074.3311	Ø 3.3 mm, L 11 mm	30	
J5074.3313	Ø 3.3 mm, L 13 mm	30	J5078.4309 Ø 4.3 mm, L 9 mm
J5074.3316	Ø 3.3 mm, L 16 mm	30	J5078.4311 Ø 4.3 mm, L 11 mm
J5074.4305	Ø 3.8/4.3 mm, L 5 mm	30	J5078.4313 Ø 4.3 mm, L 13 mm
J5074.4307	Ø 3.8/4.3 mm, L 7 mm	30	J5078.4316 Ø 4.3 mm, L 16 mm
J5074.4309	Ø 3.8/4.3 mm, L 9 mm	30	J5078.5009 Ø 5.0 mm, L 9 mm
J5074.4311	Ø 3.8/4.3 mm, L 11 mm	30	J5078.5011 Ø 5.0 mm, L 11 mm
J5074.4313	Ø 3.8/4.3 mm, L 13 mm	30	J5078.5013 Ø 5.0 mm, L 13 mm
J5074.4316	Ø 3.8/4.3 mm, L 16 mm	30	J5078.5016 Ø 5.0 mm, L 16 mm
	<b>Drill PROGRESSIVE-LINE Flex</b>		
J5074.5005	Ø 5.0 mm, L 5 mm	30	J5079.3300 Ø 3.3 mm
J5074.5007	Ø 5.0 mm, L 7 mm	30	J5079.3800 Ø 3.8 mm
J5074.5009	Ø 5.0 mm, L 9 mm	30	J5079.4300 Ø 4.3 mm
J5074.5011	Ø 5.0 mm, L 11 mm	30	J5079.5000 Ø 5.0 mm
J5074.5013	Ø 5.0 mm, L 13 mm	30	
J5074.5016	Ø 5.0 mm, L 16 mm	30	<b>Profile drill PROGRESSIVE-LINE Flex</b>
	<b>Guide System pre-drill PROGRESSIVE-LINE</b>		J5080.3300 Ø 3.3 mm
J5076.3305	Ø 3.3 mm	31	J5080.3800 Ø 3.8 mm
J5076.3805	Ø 3.8 mm	31	J5080.4300 Ø 4.3 mm
J5076.4305	Ø 4.3 mm	31	J5080.5000 Ø 5.0 mm
J5076.5005	Ø 5.0 mm	31	
	<b>Guide System form drill</b>		<b>Driver for straight bar abutment</b>
	<b>PROGRESSIVE-LINE</b>		J5300.0020 Ø 3.3/3.8/4.3 mm, short
J5076.3311	Ø 3.3 mm, L 11 mm	31	
J5076.3313	Ø 3.3 mm, L 13 mm	31	<b>Removal adapter for</b>
J5076.3316	Ø 3.3 mm, L 16 mm	31	<b>CAMLOG® and CONELOG®</b>
J5076.3809	Ø 3.8 mm, L 9 mm	31	J5300.0022 Ø 3.3/3.8/4.3/5.0 mm
J5076.3811	Ø 3.8 mm, L 11 mm	31	
J5076.3813	Ø 3.8 mm, L 13 mm	31	<b>Driver for straight bar abutment</b>
J5076.3816	Ø 3.8 mm, L 16 mm	31	J5300.0021 Ø 3.3/3.8/4.3 mm, long
J5076.4309	Ø 4.3 mm, L 9 mm	31	J5300.0025 Ø 5.0 mm, short
J5076.4311	Ø 4.3 mm, L 11 mm	31	
J5076.4313	Ø 4.3 mm, L 13 mm	31	<b>Driver for impression cap and</b>
J5076.4316	Ø 4.3 mm, L 16 mm	31	<b>healing cap for bar abutment</b>
J5076.5009	Ø 5.0 mm, L 9 mm	31	J5300.0027 Ø 3.3/3.8/4.3 mm
J5076.5011	Ø 5.0 mm, L 11 mm	31	J5300.0028 Ø 5.0 mm

# Index Article number

J5300.0030	PickUp instrument	47		Screwdriver, hex	
	Driver for screw Implants		J5317.0501	short, manual/wrench	48, 82
J5300.0031	extra short, manual/wrench	46	J5317.0502	long, manual/wrench	48, 83
J5300.0032	short, manual/wrench	46	J5317.0503	long, ISO shaft	49, 83
J5300.0033	long, manual/wrench	46	J5317.0504	short, ISO shaft	49, 83
	with ISO-shaft for angled hand piece		J5317.0510	extra short, manual/wrench	48, 82
J5300.0034	short, (with hexagon at the shaft)	46	J5317.0511	Manual screwdriver, hex	49, 83
J5300.0035	long, (with hexagon at the shaft)	46			
J5300.0036	short, (without hexagon at the shaft)	46	J5320.1030	Torque wrench	80
J5300.0037	long, (without hexagon at the shaft)	46			
J5300.0038	Cardanic driver	47	J5322.0010	Tap adapter	
			J5322.0011	short	45
				long	45
	Surgery set CAMLOG®/CONELOG®				
J5300.0063	SCREW-LINE	38	J5330.8500	Prosthetic tray	82
J5300.0065	PROGRESSIVE-LINE	22			
J5300.0071	PROGRESSIVE-LINE Flex	26	J5330.8600	Prosthetic set	82
	Pattern for surgery wash tray		J5330.8700	Prosthetic tray universal	82
	CAMLOG®/CONELOG®				
J5300.1068	SCREW-LINE	38		Pre-Osteotome SCREW-LINE,	
J5300.1070	PROGRESSIVE-LINE	22	J5417.2800	1.7 – 2.8 mm, straight convex	50, 51
	Paralleling pin			Osteotomy set	
J5300.2000	PROGRESSIVE-LINE	23		CAMLOG®/CONELOG® SCREW-LINE,	
J5300.2028	SCREW-LINE	45	J5418.0020	straight convex	50
			J5418.0030	angled convex	51
	Surgery tray				
	CAMLOG®/CONELOG® (without content)			Osteotome SCREW-LINE	
J5300.8916	SCREW-LINE	38	J5418.3300	Ø 3.3 mm, straight convex	50
J5300.8917	PROGRESSIVE-LINE	22	J5418.3310	Ø 3.3 mm, angled convex	51
J5300.8920	PROGRESSIVE-LINE Flex	26	J5418.3800	Ø 3.8 mm, straight convex	50
			J5418.3810	Ø 3.8 mm, angled convex	51
	Guide System surgery tray		J5418.4300	Ø 4.3 mm, straight convex	50
	CAMLOG®/CONELOG® (without content)		J5418.4310	Ø 4.3 mm, angled convex	51
J5300.8919	PROGRESSIVE-LINE	30	J5418.5000	Ø 5.0 mm, straight convex	50
			J5418.5010	Ø 5.0 mm, angled convex	51
	Surgery wash tray		J5418.6000	Ø 6.0 mm, straight convex	50
	CAMLOG®/CONELOG® (without content)		J5418.6010	Ø 6.0 mm, angled convex	51
J5300.8968	SCREW-LINE	38			
J5300.8970	PROGRESSIVE-LINE	22		Pre-Osteotome SCREW-LINE	
			J5419.2800	1.7 – 2.8 mm, straight concave	52, 53
	Guide System Check-up pin				
J5301.3300	Ø 3.3 mm	42		Osteotomy set	
J5301.3310	Ø 3.3 mm, PROGRESSIVE-LINE	32		CAMLOG®/CONELOG® SCREW-LINE,	
J5301.4300	Ø 3.8/4.3 mm	42	J5420.0020	straight concave	52
J5301.4310	Ø 3.8/4.3 mm, PROGRESSIVE-LINE	32	J5420.0030	angled concave	53
J5301.5010	Ø 5.0 mm, PROGRESSIVE-LINE	32		Osteotomy SCREW-LINE	
J5302.0010	Holding key for insertion post	48	J5420.3300	Ø 3.3 mm, straight concave	52
			J5420.3310	Ø 3.3 mm, angled concave	53
	Holding sleeve for screw Implants		J5420.3800	Ø 3.8 mm, straight concave	52
J5302.3300	Ø 3.3 mm	48	J5420.3810	Ø 3.8 mm, angled concave	53
J5302.3800	Ø 3.8 mm	48	J5420.4300	Ø 4.3 mm, straight concave	52
J5302.4300	Ø 4.3 mm	48	J5420.4310	Ø 4.3 mm, angled concave	53
J5302.5000	Ø 5.0 mm	48	J5420.5000	Ø 5.0 mm, straight concave	52
J5302.6000	Ø 6.0 mm	48	J5420.5010	Ø 5.0 mm, angled concave	53
			J5420.6000	Ø 6.0 mm, straight concave	52
			J5420.6010	Ø 6.0 mm, angled concave	53

J8070.2050	Edentulous mandible	89	SCREW-LINE Implant, Promote® plus incl. snap-in insertion post	
	SCREW-LINE Implant, Promote® incl. screw-mounted insertion post		K1056.3311	Ø 3.3 mm, L 11 mm
			K1056.3313	Ø 3.3 mm, L 13 mm
K1045.3311	Ø 3.3 mm, L 11 mm	35	K1056.3316	Ø 3.3 mm, L 16 mm
K1045.3313	Ø 3.3 mm, L 13 mm	35	K1056.3809	Ø 3.8 mm, L 9 mm
K1045.3316	Ø 3.3 mm, L 16 mm	35	K1056.3811	Ø 3.8 mm, L 11 mm
K1045.3809	Ø 3.8 mm, L 9 mm	35	K1056.3813	Ø 3.8 mm, L 13 mm
K1045.3811	Ø 3.8 mm, L 11 mm	35	K1056.3816	Ø 3.8 mm, L 16 mm
K1045.3813	Ø 3.8 mm, L 13 mm	35	K1056.4309	Ø 4.3 mm, L 9 mm
K1045.3816	Ø 3.8 mm, L 16 mm	35	K1056.4311	Ø 4.3 mm, L 11 mm
K1045.4309	Ø 4.3 mm, L 9 mm	35	K1056.4313	Ø 4.3 mm, L 13 mm
K1045.4311	Ø 4.3 mm, L 11 mm	35	K1056.4316	Ø 4.3 mm, L 16 mm
K1045.4313	Ø 4.3 mm, L 13 mm	35	K1056.5009	Ø 5.0 mm, L 9 mm
K1045.4316	Ø 4.3 mm, L 16 mm	35	K1056.5011	Ø 5.0 mm, L 11 mm
K1045.5009	Ø 5.0 mm, L 9 mm	35	K1056.5013	Ø 5.0 mm, L 13 mm
K1045.5011	Ø 5.0 mm, L 11 mm	35	K1056.5016	Ø 5.0 mm, L 16 mm
K1045.5013	Ø 5.0 mm, L 13 mm	35	K1056.6009	Ø 6.0 mm, L 9 mm
	SCREW-LINE Implant, Promote® incl. snap-in insertion post		K1056.6011	Ø 6.0 mm, L 11 mm
			K1056.6013	Ø 6.0 mm, L 13 mm
			K1056.6016	Ø 6.0 mm, L 16 mm
K1046.3311	Ø 3.3 mm, L 11 mm	34		
K1046.3313	Ø 3.3 mm, L 13 mm	34		
K1046.3316	Ø 3.3 mm, L 16 mm	34		
K1046.3809	Ø 3.8 mm, L 9 mm	34	K1075.3311	Ø 3.3 mm, L 11 mm
K1046.3811	Ø 3.8 mm, L 11 mm	34	K1075.3313	Ø 3.3 mm, L 13 mm
K1046.3813	Ø 3.8 mm, L 13 mm	34	K1075.3316	Ø 3.3 mm, L 16 mm
K1046.3816	Ø 3.8 mm, L 16 mm	34	K1075.3809	Ø 3.8 mm, L 9 mm
K1046.4309	Ø 4.3 mm, L 9 mm	34	K1075.3811	Ø 3.8 mm, L 11 mm
K1046.4311	Ø 4.3 mm, L 11 mm	34	K1075.3813	Ø 3.8 mm, L 13 mm
K1046.4313	Ø 4.3 mm, L 13 mm	34	K1075.3816	Ø 3.8 mm, L 16 mm
K1046.4316	Ø 4.3 mm, L 16 mm	34	K1075.4309	Ø 4.3 mm, L 9 mm
K1046.5009	Ø 5.0 mm, L 9 mm	34	K1075.4311	Ø 4.3 mm, L 11 mm
K1046.5011	Ø 5.0 mm, L 11 mm	34	K1075.4313	Ø 4.3 mm, L 13 mm
K1046.5013	Ø 5.0 mm, L 13 mm	34	K1075.4316	Ø 4.3 mm, L 16 mm
K1046.5016	Ø 5.0 mm, L 16 mm	34	K1075.5009	Ø 5.0 mm, L 9 mm
K1046.6009	Ø 6.0 mm, L 9 mm	34	K1075.5011	Ø 5.0 mm, L 11 mm
K1046.6011	Ø 6.0 mm, L 11 mm	34	K1075.5013	Ø 5.0 mm, L 13 mm
K1046.6013	Ø 6.0 mm, L 13 mm	34	K1075.5016	Ø 5.0 mm, L 16 mm
K1046.6016	Ø 6.0 mm, L 16 mm	34		
	SCREW-LINE Implant for practice			
K1049.3813	Ø 3.8 mm, L 13 mm	88	K1076.3311	Ø 3.3 mm, L 11 mm
K1049.4313	Ø 4.3 mm, L 13 mm	88	K1076.3313	Ø 3.3 mm, L 13 mm
	SCREW-LINE Implant, Promote® plus incl. screw-mounted insertion post		K1076.3316	Ø 3.3 mm, L 16 mm
K1055.3311	Ø 3.3 mm, L 11 mm	35	K1076.3809	Ø 3.8 mm, L 9 mm
K1055.3313	Ø 3.3 mm, L 13 mm	35	K1076.3811	Ø 3.8 mm, L 11 mm
K1055.3316	Ø 3.3 mm, L 16 mm	35	K1076.3813	Ø 3.8 mm, L 13 mm
K1055.3809	Ø 3.8 mm, L 9 mm	35	K1076.3816	Ø 3.8 mm, L 16 mm
K1055.3811	Ø 3.8 mm, L 11 mm	35	K1076.4309	Ø 4.3 mm, L 9 mm
K1055.3813	Ø 3.8 mm, L 13 mm	35	K1076.4311	Ø 4.3 mm, L 11 mm
K1055.3816	Ø 3.8 mm, L 16 mm	35	K1076.4313	Ø 4.3 mm, L 13 mm
K1055.4309	Ø 4.3 mm, L 9 mm	35	K1076.4316	Ø 4.3 mm, L 16 mm
K1055.4311	Ø 4.3 mm, L 11 mm	35	K1076.5009	Ø 5.0 mm, L 9 mm
K1055.4313	Ø 4.3 mm, L 13 mm	35	K1076.5011	Ø 5.0 mm, L 11 mm
K1055.4316	Ø 4.3 mm, L 16 mm	35	K1076.5013	Ø 5.0 mm, L 13 mm
K1055.5009	Ø 5.0 mm, L 9 mm	35	K1076.5016	Ø 5.0 mm, L 16 mm
K1055.5011	Ø 5.0 mm, L 11 mm	35		
K1055.5013	Ø 5.0 mm, L 13 mm	35		

# Index Article number

	PROGRESSIVE-LINE Implant for practice			Impression posts, open tray	
K1901.3813	Ø 3.8 mm, L 13 mm	88	K2121.3300	Ø 3.3 mm	60
K1901.4313	Ø 4.3 mm, L 13 mm	88	K2121.3800	Ø 3.8 mm	60
	Healing cap PS		K2121.4300	Ø 4.3 mm	60
K2001.3840	Ø 3.8 mm, GH 4.0 mm, bottleneck	58	K2121.5000	Ø 5.0 mm	60
K2001.3860	Ø 3.8 mm, GH 6.0 mm, bottleneck	58	K2121.6000	Ø 6.0 mm	60
K2001.4340	Ø 4.3 mm, GH 4.0 mm, bottleneck	58		Universal abutments PS	
K2001.4360	Ø 4.3 mm, GH 6.0 mm, bottleneck	58	K2201.3800	Ø 3.8 mm	67, 79
K2001.5040	Ø 5.0 mm, GH 4.0 mm, bottleneck	58	K2201.4300	Ø 4.3 mm	67, 79
K2001.5060	Ø 5.0 mm, GH 6.0 mm, bottleneck	58	K2201.5000	Ø 5.0 mm	67, 79
K2004.3840	Ø 3.8 mm, GH 4.0 mm, wide body	58	K2201.6000	Ø 6.0 mm	67, 79
K2004.3860	Ø 3.8 mm, GH 6.0 mm, wide body	58		Esthomic® Abutments PS, straight, for Platform Switching	
K2004.4340	Ø 4.3 mm, GH 4.0 mm, wide body	58			
K2004.4360	Ø 4.3 mm, GH 6.0 mm, wide body	58	K2202.3815	Ø 3.8 mm	63
K2004.5040	Ø 5.0 mm, GH 4.0 mm, wide body	58	K2202.4315	Ø 4.3 mm	63
K2004.5060	Ø 5.0 mm, GH 6.0 mm, wide body	58	K2202.5015	Ø 5.0 mm	63
K2004.6040	Ø 6.0 mm, GH 4.0 mm, wide body	58	K2202.6015	Ø 6.0 mm	63
K2004.6060	Ø 6.0 mm, GH 6.0 mm, wide body	58		Temporary abutments PS, PEEK, for Platform Switching	
K2005.3820	Ø 3.8 mm, GH 2.0 mm, cylindrical	58			
K2005.3840	Ø 3.8 mm, GH 4.0 mm, cylindrical	58	K2203.3815	Ø 3.8 mm, type A	63
K2005.3860	Ø 3.8 mm, GH 6.0 mm, cylindrical	58	K2203.4315	Ø 4.3 mm, type A	63
K2005.4320	Ø 4.3 mm, GH 2.0 mm, cylindrical	58	K2203.5015	Ø 5.0 mm, type A	63
K2005.4340	Ø 4.3 mm, GH 4.0 mm, cylindrical	58	K2203.6015	Ø 6.0 mm, type A	63
K2005.4360	Ø 4.3 mm, GH 6.0 mm, cylindrical	58	K2204.3815	Ø 3.8 mm, type B	63
K2005.5020	Ø 5.0 mm, GH 2.0 mm, cylindrical	58	K2204.4315	Ø 4.3 mm, type B	63
K2005.5040	Ø 5.0 mm, GH 4.0 mm, cylindrical	58	K2204.5015	Ø 5.0 mm, type B	63
K2005.5060	Ø 5.0 mm, GH 6.0 mm, cylindrical	58	K2204.6015	Ø 6.0 mm, type B	63
K2005.6020	Ø 6.0 mm, GH 2.0 mm, cylindrical	58		Titanium base CAD/CAM PS for Platform Switching, crown	
K2005.6040	Ø 6.0 mm, GH 4.0 mm, cylindrical	58	K2210.3808	Ø 3.8 mm	64
K2005.6060	Ø 6.0 mm, GH 6.0 mm, cylindrical	58	K2210.4308	Ø 4.3 mm	64
	Guide System CAMLOG® Insertion post, screw-mounted		K2210.5008	Ø 5.0 mm	64
K2026.3303	Ø 3.3 mm	32, 42	K2208.3800	Ø 3.8 mm	62
K2026.3803	Ø 3.8 mm	32, 42	K2208.4300	Ø 4.3 mm	62
K2026.4303	Ø 4.3 mm	32, 42	K2208.5000	Ø 5.0 mm	62
K2026.5003	Ø 5.0 mm	32	K2208.6000	Ø 6.0 mm	62
	Impression posts PS, closed tray, for Platform Switching			Universal abutments	
K2109.3800	Ø 3.8 mm	60	K2211.3300	Ø 3.3 mm	67
K2109.4300	Ø 4.3 mm	60	K2211.3800	Ø 3.8 mm	67, 79
K2109.5000	Ø 5.0 mm	60	K2211.4300	Ø 4.3 mm	67, 79
K2109.6000	Ø 6.0 mm	60	K2211.5000	Ø 5.0 mm	67, 79
	Impression posts, closed tray		K2211.6000	Ø 6.0 mm	67, 79
K2110.3300	Ø 3.3 mm	60		Telescope abutments for double crown restorations	
K2110.3800	Ø 3.8 mm	60	K2212.3800	Ø 3.8 mm	79
K2110.4300	Ø 4.3 mm	60	K2212.4300	Ø 4.3 mm	79
K2110.5000	Ø 5.0 mm	60	K2212.5000	Ø 5.0 mm	79
K2110.6000	Ø 6.0 mm	60	K2212.6000	Ø 6.0 mm	79
	Impression posts PS, open tray, for Platform Switching				
K2119.3800	Ø 3.8 mm	60			
K2119.4300	Ø 4.3 mm	60			
K2119.5000	Ø 5.0 mm	60			
K2119.6000	Ø 6.0 mm	60			

	<b>Esthomic® Abutments, straight</b>			<b>Temporary abutments, PEEK</b>	
K2226.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm	62	K2241.3800	Ø 3.8 mm	62
K2226.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	62	K2241.4300	Ø 4.3 mm	62
K2226.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm	62	K2241.5000	Ø 5.0 mm	62
K2226.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	62	K2241.6000	Ø 6.0 mm	62
K2226.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm	62			
K2226.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	62		Titanium bases CAD/CAM, crown	
K2226.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm	62	K2244.3348	Ø 3.3 mm	64
K2226.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm	62	K2244.3848	Ø 3.8 mm	64
	<b>Esthomic® Abutments, 15° angled</b>		K2244.4348	Ø 4.3 mm	64
K2227.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm, type A	62	K2244.5048	Ø 5.0 mm	64
K2227.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm, type A	62	K2244.6048	Ø 6.0 mm	64
K2227.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm, type A	62		<b>Gold-plastic abutment</b>	
K2227.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm, type A	62	K2246.3300	Ø 3.3 mm	67
K2227.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm, type A	62	K2246.3800	Ø 3.8 mm	67
K2227.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm, type A	62	K2246.4300	Ø 4.3 mm	67
K2227.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm, type A	62	K2246.5000	Ø 5.0 mm	67
K2227.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm, type A	62	K2246.6000	Ø 6.0 mm	67
K2228.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm, type B	63			
K2228.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm, type B	63		<b>Bar abutment, 17° angled</b>	
K2228.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm, type B	63	K2256.3325	Ø 3.3 mm, GH 2.5, type A	69
K2228.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm, type B	63	K2256.3340	Ø 3.3 mm, GH 4.0, type A	69
K2228.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm, type B	63	K2256.3825	Ø 3.8 mm, GH 2.5, type A	69
K2228.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm, type B	63	K2256.3840	Ø 3.8 mm, GH 4.0, type A	69
K2228.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm, type B	63	K2256.4325	Ø 4.3 mm, GH 2.5, type A	69
K2228.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm, type B	63	K2256.4340	Ø 4.3 mm, GH 4.0, type A	69
	<b>Esthomic® Abutments, 20° angled</b>		K2256.5025	Ø 5.0 mm, GH 2.5, type A	69
K2231.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm, type A	63	K2256.5040	Ø 5.0 mm, GH 4.0, type A	69
K2231.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm, type A	63	K2257.3325	Ø 3.3 mm, GH 2.5, type B	69
K2231.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm, type A	63	K2257.3340	Ø 3.3 mm, GH 4.0, type B	69
K2231.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm, type A	63	K2257.3825	Ø 3.8 mm, GH 2.5, type B	69
K2231.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm, type A	63	K2257.3840	Ø 3.8 mm, GH 4.0, type B	69
K2231.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm, type A	63	K2257.4325	Ø 4.3 mm, GH 2.5, type B	69
K2231.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm, type A	63	K2257.4340	Ø 4.3 mm, GH 4.0, type B	69
K2231.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm, type A	63	K2257.5025	Ø 5.0 mm, GH 2.5, type B	69
K2231.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm, type B	63	K2257.5040	Ø 5.0 mm, GH 4.0, type B	69
K2232.3810	Ø 3.8 mm, GH 1.0 – 1.8 mm, type B	63			
K2232.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm, type B	63		<b>Bar abutment, 30° angled</b>	
K2232.4310	Ø 4.3 mm, GH 1.0 – 1.8 mm, type B	63	K2258.3325	Ø 3.3 mm, GH 2.5, type A	69
K2232.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm, type B	63	K2258.3340	Ø 3.3 mm, GH 4.0, type A	69
K2232.5010	Ø 5.0 mm, GH 1.0 – 1.8 mm, type B	63	K2258.3825	Ø 3.8 mm, GH 2.5, type A	69
K2232.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm, type B	63	K2258.3840	Ø 3.8 mm, GH 4.0, type A	69
K2232.6010	Ø 6.0 mm, GH 1.0 – 1.8 mm, type B	63	K2258.4325	Ø 4.3 mm, GH 2.5, type A	69
K2232.6030	Ø 6.0 mm, GH 3.0 – 4.5 mm, type B	63	K2258.4340	Ø 4.3 mm, GH 4.0, type A	69
	<b>Esthomic® Abutments, Inset</b>		K2258.5035	Ø 5.0 mm, GH 3.5, type A	69
K2235.3315	Ø 3.3 mm, GH 1.5 – 2.8 mm	63	K2258.5050	Ø 5.0 mm, GH 5.0, type A	69
K2235.3815	Ø 3.8 mm, GH 1.5 – 2.8 mm	63	K2259.3325	Ø 3.3 mm, GH 2.5, type B	69
K2235.4315	Ø 4.3 mm, GH 1.5 – 2.8 mm	63	K2259.3340	Ø 3.3 mm, GH 4.0, type B	69
K2235.5015	Ø 5.0 mm, GH 1.5 – 2.8 mm	63	K2259.3825	Ø 3.8 mm, GH 2.5, type B	69
K2235.6015	Ø 6.0 mm, GH 1.5 – 2.8 mm	63	K2259.3840	Ø 3.8 mm, GH 4.0, type B	69
	<b>Temporary abutment, crown, titanium alloy</b>		K2259.4325	Ø 4.3 mm, GH 2.5, type B	69
K2239.3300	Ø 3.3 mm	62	K2259.4340	Ø 4.3 mm, GH 4.0, type B	69
K2239.3800	Ø 3.8 mm	62	K2259.5035	Ø 5.0 mm, GH 3.5, type B	69
K2239.4300	Ø 4.3 mm	62	K2259.5050	Ø 5.0 mm, GH 5.0, type B	69
K2239.5000	Ø 5.0 mm	62			
K2239.6000	Ø 6.0 mm	62			

# Index Article number

	CAM Titanium Blank		K5300.9010	X-Ray Planning foil 1.25:1	16
K2411.3313	Ø 3.3 mm, type IAC	66	K5300.9011	X-Ray Planning foil 1.4:1	16
K2411.3813	Ø 3.8 mm, type IAC	66		CAMLOG® SCREW-LINE Implants	
K2411.4313	Ø 4.3 mm, type IAC	66			
K2411.6013	Ø 5.0/6.0 mm, type IAC	66	K5300.9014	X-Ray Planning foil 1.25:1	16
K2421.3320	Ø 3.3 mm, type ME	66	K5300.9015	X-Ray Planning foil 1.4:1	16
K2421.3820	Ø 3.8 mm, type ME	66		CAMLOG® PROGRESSIVE-LINE Implants	
K2421.4320	Ø 4.3 mm, type ME	66			
K2421.5020	Ø 5.0 mm, type ME	66		X-Ray Transfer pictures 1.25:1	
K2421.6020	Ø 6.0 mm, type ME	66		CAMLOG® SCREW-LINE Implants	
	Logfit® Abutments		K5300.9080	Ø 3.3 mm	16
K2550.3808	Ø 3.8 mm, GH 0.8 mm	68	K5300.9081	Ø 3.8 mm	16
K2550.3815	Ø 3.8 mm, GH 1.5 mm	68	K5300.9082	Ø 4.3 mm	16
K2550.4308	Ø 4.3 mm, GH 0.8 mm	68	K5300.9083	Ø 5.0 mm	16
K2550.4315	Ø 4.3 mm, GH 1.5 mm	68	K5300.9084	Ø 6.0 mm	16
K2550.5008	Ø 5.0 mm, GH 0.8 mm	68		Adapter for screw Implants	
K2550.5015	Ø 5.0 mm, GH 1.5 mm	68	K5302.3310	Ø 3.3 mm, long	48
K2550.6008	Ø 6.0 mm, GH 0.8 mm	68	K5302.3311	Ø 3.3 mm, short	48
K2550.6015	Ø 6.0 mm, GH 1.5 mm	68	K5302.3810	Ø 3.8 mm, long	48
	Scanbodies		K5302.3811	Ø 3.8 mm, short	48
K2610.3310	Ø 3.3 mm	65	K5302.4310	Ø 4.3 mm, long	48
K2610.3810	Ø 3.8 mm	65	K5302.4311	Ø 4.3 mm, short	48
K2610.4310	Ø 4.3 mm	65	K5302.6011	Ø 5.0/6.0 mm, short	48
K2610.6010	Ø 5.0/6.0 mm	65		Macro model	
	ScanPosts for Sirona® Scanbody		K8010.1010	SCREW-LINE	89
K2620.3306	Ø 3.3 mm	65	K8010.1400	PROGRESSIVE-LINE	89
K2620.3806	Ø 3.8 mm	65	K8011.1000	Selection abutment kit	85
K2620.4306	Ø 4.3 mm	65			
K2620.5006	Ø 5.0 mm	65		Demonstration model, acrylic glass	
K2620.6006	Ø 6.0 mm	65	K8050.1040	Lower jaw	89
	Lab analog		K8070.1020	Upper jaw	89
K3010.3300	Ø 3.3 mm	61	M1000.0050	ALTApin magazine, 1 unit	56
K3010.3800	Ø 3.8 mm	61	M1000.0100	ALTApin magazine, 3 units	56
K3010.4300	Ø 4.3 mm	61			
K3010.5000	Ø 5.0 mm	61	M5100.0010	ALTApin applicator, straight	54
K3010.6000	Ø 6.0 mm	61	M5100.0030	ALTApin applicator, angled 90°	54
	DIM Analog® for the CAMLOG® Implant System		M5100.0050	ALTApin pricker	55
K3012.3300	Ø 3.3 mm	61	M5100.0070	ALTApin membrane fixator	55
K3012.3800	Ø 3.8 mm	61			
K3012.4300	Ø 4.3 mm	61	M5100.0100	ALTApin surgery mallet	55
K3012.6000	Ø 5.0/6.0 mm	61			
	Implant analog		M5200.0010	ALTApin Applicator, straight, work element	54
K3025.3300	Ø 3.3 mm	61			
K3025.3800	Ø 3.8 mm	61	M5200.0055	ALTApin pricker, insert	56
K3025.4300	Ø 4.3 mm	61			
K3025.5000	Ø 5.0 mm	61	M5500.0050	ALTApin single patient drill, ISO shaft	55
K3025.6000	Ø 6.0 mm	61			
	Collet for CAM Blank, type IAC		M5600.0110	ALTApin set	54
K3720.3300	Ø 3.3 mm	66	M5600.0210	ALTApin tray	54
K3720.3800	Ø 3.8 mm	66			
K3720.4300	Ø 4.3 mm	66			
K3720.6000	Ø 5.0/6.0 mm	66			

# Further documentation

Further information on the CAMLOG® Products can be found in the following documents:

- CAMLOG® Product catalog
- CAMLOG® Working instructions
- CAMLOG® Instruction for use
- Preparation instructions
- Camlog literature overview
- Camlog and science

The documents are available from the local Camlog representative.

See also:

<https://ifu.camlog.com>

[www.camlog.com](http://www.camlog.com)

## References

- [1] Conserva E. Initial stability after placement of a new buttress threaded implant. A case series study. implants. 2019(3): 24-28.
- [2] Ruppin J. One-year clinical experience with Progressive-Line implants. EDI journal. 2020(4): 54-63.
- [3] Semper-Hogg W, Kraft S, Stiller S, Mehrhof J, Nelson K. Analytical and experimental position stability of the abutment in different dental implant systems with a conical implant-abutment connection. Clin Oral Investig 2010;17(3): 1017-23.
- [4] Semper Hogg W, Zulauf K, Mehrhof J, Nelson K. The influence of torque tightening on the position stability of the abutment in conical implant-abutment connections. Int J Prosthodont 2015;28: 538-41.

## Trademarks and copyright

Protected trade names (trademarks) are not always specially indicated. The absence of such an indication does not mean that this name is NOT a trademark. The document including all its parts is protected by copyright. You may download the content regarding the intended use, but changes to or reproduction of the content are not permitted. Any exploitation beyond the narrow limits of the copyright act is not permitted without prior written approval of CAMLOG Biotechnologies GmbH and is subject to legal sanctions.

CE 0123



+E219480010003D



+\$0090113102DO

Art. No. J8001.0003 Rev. 09 07/2021

#### Headquarters

CAMLOG Biotechnologies GmbH | Margarethenstr. 38 | 4053 Basel | Switzerland  
Phone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.camlog.com

Manufacturer CAMLOG® and CONELOG® Products: ALTATEC GmbH | Maybachstr. 5 | 71299 Wimsheim | Germany

