



Product catalog
CONELOG® Implant System

Valid from August 2020



Content

System information

The CONELOG® Implant System	2
-----------------------------	---

Surgery

Planning	16
PROGRESSIVE-LINE Implants and instruments	19
PROGRESSIVE-LINE Flex instruments	24
PROGRESSIVE-LINE Guide System	28
SCREW-LINE Implants and instruments	33
SCREW-LINE Guide System Implants and instruments	38
General surgical instruments	42
Osteotomy set	49
ALTApin set	53
Cover screws	55
Healing caps	55

Prosthetics

Impression taking	58
Bite registration	59
Fabrication of the plaster model	59
Temporary restoration	60
Esthomic® Abutments	60
CAD/CAM prosthetics	62
CAM titanium blanks	64
Universal abutments	65
Gold-plastic abutment	65
Logfit® Prosthetic system	66
COMFOUR® System	67
Ball abutment anchoring system	71
Locator® Anchoring system	72
Double crown restorations	77
Accessories for abutments	77
Prosthetic instruments	78
Instruments for dental technicians	82
Selection abutments	83

Auxiliary article

Implants for practice	86
Demonstration models	87
Macro models	87
Literature	88

Auxiliary information

Indication overview	90
Implant overview	93
Prosthetics overview	94
Screw overview	100
Overview tightening torque	104
Materials	106

Index

Alphabetical	108
Article number	112
Further documentation	122

The CONELOG® Implant System



The CONELOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, consistent prosthetically oriented implant system.

All CONELOG® Products are manufactured with the latest state-of-the-art technology. The CONELOG® Implant System is continuously being developed by the company's research and development team in collaboration with clinics, universities and dental technicians and therefore stays abreast of the latest technology.

The CAMLOG® and CONELOG® Implant Systems are very well documented scientifically. Studies* support this with respect to a great many parameters including the implant surface, time of implantation and/or implant loading, primary stability, and the connection design. The long-term results of the Promote® Surface are convincing.

The descriptions that follow are not adequate to permit immediate use of the CONELOG® Implant System.

Instruction by a surgeon experienced in using the system is strongly recommended. CONELOG® Products should only be used by dentists, doctors, surgeons and dental technicians who have been trained in using the system. Appropriate courses and training sessions are regularly offered by Camlog.

Methodological errors in treatment can result in loss of the implant and significant loss of peri-implant bone.

Not all products and services from Camlog are available in all countries.

Packaging units: unless described otherwise, each pack contains one product.

The images in this document are for reference purposes only and may differ from the actual product.

* See «Further documentation» on page 122

CONELOG® PROGRESSIVE-LINE Implants

The new CONELOG® PROGRESSIVE-LINE Implants make it easier to implement modern treatment concepts such as immediate restorations or immediate loading, which require high primary stability [1, 2]*.

The geometry of the implant is consistently designed to develop high initial stability:

- The self-tapping screw implant has a conically shaped apical area that enables pronounced primary stability even in soft bone [1, 2]*.
- Thread extending to the apex for good anchorage in immediate implantations [1, 2]*.
- Crestal thread for improved hold with limited bone height [2]*.

CONELOG® PROGRESSIVE-LINE Implants are available with the abrasive-blasted, acid-etched Promote® Surface which extends over the entire implant body up to the acid-etched conical 45° implant shoulder. Depending on the clinical situation, this surface design thus permits epicrestal or slightly subcrestal implant positioning in the sense of a classic bone level implant.

PROGRESSIVE-LINE Implants with screw-mounted insertion post can be used for the guided implantation.


CONELOG® PROGRESSIVE-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.



CONELOG® PROGRESSIVE-LINE
Implant Promote® plus

* see «Further documentation» on page 122.

Implant diameters



3.3 mm 3.8 mm 4.3 mm 5.0 mm

Implant lengths



7 mm 9 mm 11 mm 13 mm 16 mm



CONELOG® SCREW-LINE
Implant Promote® plus

CONELOG® SCREW-LINE Implants


CONELOG® SCREW-LINE Implants are slightly conical, self-tapping screw implants. They enable easy insertion by self-centering with continuous bone contact to achieve solid primary stability.

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® surface up to the acid-etched conical 45° implant shoulder and thus allow for maximum flexibility when determining the vertical implant position. Rounding of the apical geometry ensures gentle insertion of the CONELOG® SCREW-LINE Implants into the bone, also near the maxillary sinus.

SCREW-LINE Implants with screw-mounted insertion post can be used for the guided implantation.

CONELOG® SCREW-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.

Implant diameters



3.3 mm 3.8 mm 4.3 mm 5.0 mm

Implant lengths



7 mm 9 mm 11 mm 13 mm 16 mm

All CONELOG® Implants are delivered pre-assembled in sterile packaging on a color-coded insertion post corresponding to the diameter.

CONELOG® Implant-Abutment connection

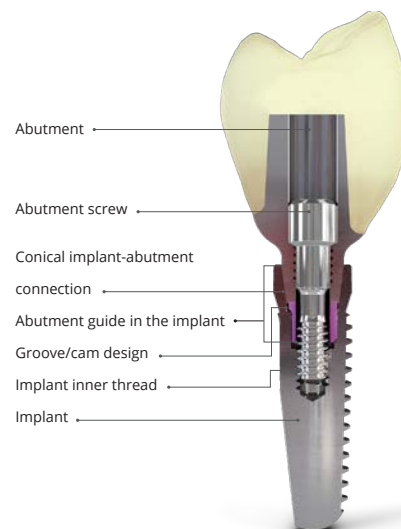
The geometry of the CONELOG® Implant-Abutment connection enables integrated Platform Switching and provides excellent tactile feedback when inserting the abutments. Indexing via the three grooves/cams allows the cams to slide noticeably into the grooves of the implant and thus into the final position when the abutment is rotated slightly. Simple, easy and safe orientation in the longitudinal axis of the implant is thus ensured. The precise conical connection minimizes micro-movements and demonstrates superior stability compared to other conical connections [3, 4]*.

* See „Further documentation“ on page 122

Advantages and benefits of the CONELOG® Connection

- Simple, fast and precise abutment positioning with clearly noticeable tactile feedback
- Precise, conical implant-abutment connection with superior stability compared to other conical connections
- Integrated Platform Switching

For optimal positioning of the abutments, the implant should be aligned in the bone so that one of the three grooves points in vestibular direction. With the CONELOG® Implants, the insertion tools include markings that correspond to the three grooves of the implant inner configuration.



Promote® Surface

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface. The surface is based on current scientific knowledge and supports rapid osseointegration. Scientific results from studies with cell cultures, osteohistology and in pull-out trials illustrate this impressively.



Production precision

The inner and outer geometry of the CONELOG® Implants and abutments are rotary machined for the most part. The tolerances can therefore be kept very low. The result is excellent part precision without impacting the material structure. The CONELOG® Implant-abutment connection thus ensures a very precise, stable and rotation-locked connection to the prosthetic components.

CONELOG® Prosthetic components

The CONELOG® SCREW-LINE Implants can be provided with a wide range of flexible, anatomically adapted prosthetic components. CONELOG® Abutments are color-coded according to the implant diameters.

Effect of the Platform Switching design

The CONELOG® Implant system offers integrated Platform Switching as the implant shoulder is not covered by the healing caps and abutments. Platform Switching option is used to support the hard and soft tissue in the peri-implant esthetic region. The distance between the implant-abutment interface and the alveolar crest is increased and thereby reduces the effect of inflammatory cell infiltration with concomitant bone resorption.



CONELOG® Healing caps

CONELOG® Healing caps sit on the machined implant shoulder, but do not cover it completely. As a result, the soft tissue over the shoulder can be adapted. The conical surfaces do not come into contact.

The healing caps are used according to indication for single and two-stage procedures. The healing caps are available in three geometries (cylindrical, wide body and bottleneck) and are screwed directly into the implant.

CONELOG® Impression taking

Impression-taking of the CONELOG® Implants is possible with impression posts, open or closed tray. All impression-taking components are color-coded based on the implant diameter. High-precision components ensure correct transfer of the intraoral situation.

The CONELOG® Impression posts do not lock into the cone of the implant, but lie on the implant shoulder. Thus, a vertical offset is prevented when taking the impression. The antirotational mechanism is ensured by the CONELOG® Groove/cam geometry.





CONELOG® Temporary abutments

CONELOG® Temporary abutments made of titanium alloy are available for temporary restorations in crown and bridge versions. The abutments can be used in immediate implantations or after exposing the gingiva.

CONELOG® Titanium bases CAD/CAM

CONELOG® Titanium bases CAD/CAM are acting as a bonding basis for customized, implant-supported dental restorations made of suitable materials. Reconstructions are fabricated with the aid of CAD/CAM techniques. CONELOG® Titanium bases CAD/CAM are available in crown and bridge versions in the gingival heights 0.8 and 2.0 mm.

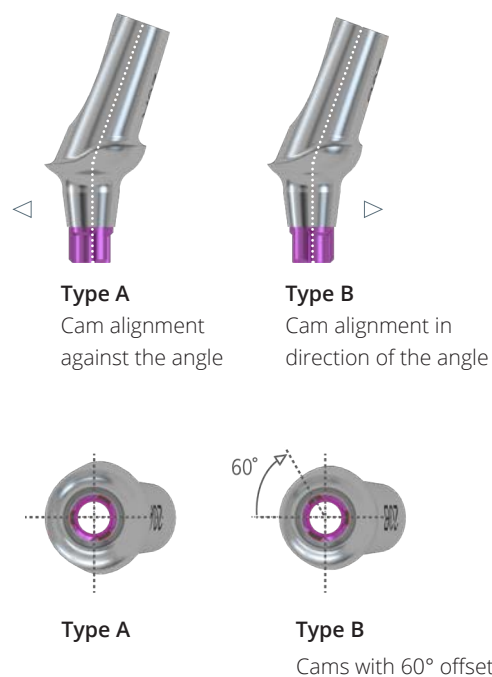


CONELOG® Esthomic® Abutments

Anatomically preformed abutments allow for optimal stump design. The CONELOG® Esthomic® Abutments are available both straight and angled with various gingival heights and with an oval anatomically pre-shaped shoulder profile. The angled Esthomic® Abutments are available in A and B versions differentiated by a cam offset of 60°. This results in six prosthetic-oriented rotating positions and allows perfect prosthetic alignment of the axes.



CONELOG® Esthomic® Abutment cam alignment



CONELOG® Gold-plastic abutment

The CONELOG® Gold-plastic abutment can be used with the cast-on technique to fabricate a multitude of customized implant restorations, such as single crowns, mesostructures for cementable bridge restorations and primary abutments for bridging implant axis divergences in the double crown technique.



CONELOG® Logfit® Abutments

The CONELOG® Logfit® Prosthetic System can be used for fabricating cementable crown and bridge restorations. The Logfit® Prosthetic System consists of prefabricated components precisely matched to one another and thus standardizes the clinical and technical procedure. The result is a lower workload for the practice and the dental laboratory.



CONELOG® Universal and telescope abutment

CONELOG® Universal and telescope abutments can be used for individually fabricated cementable crown and bridge restorations and for double crown restorations. The abutments are made of titanium alloy and can be custom trimmed.



CONELOG® Ball, Locator® and straight bar abutments

Ball, Locator® and straight bar abutments are available for the CONELOG® Implant System. These differ from the abutments in the apical region through different connection designs. Ball, Locator® and straight bar abutments are manufactured as single pieces with a thread in the apical region which engages with the inner thread of the CONELOG® Implant. These abutments are screwed into the CONELOG® Implant using the corresponding insertion tools.



Example: CONELOG® Ball abutment (Ø 4.3 mm) in a CONELOG® SCREW-LINE Implant

CONELOG® Disconnecter for CONELOG® Abutments

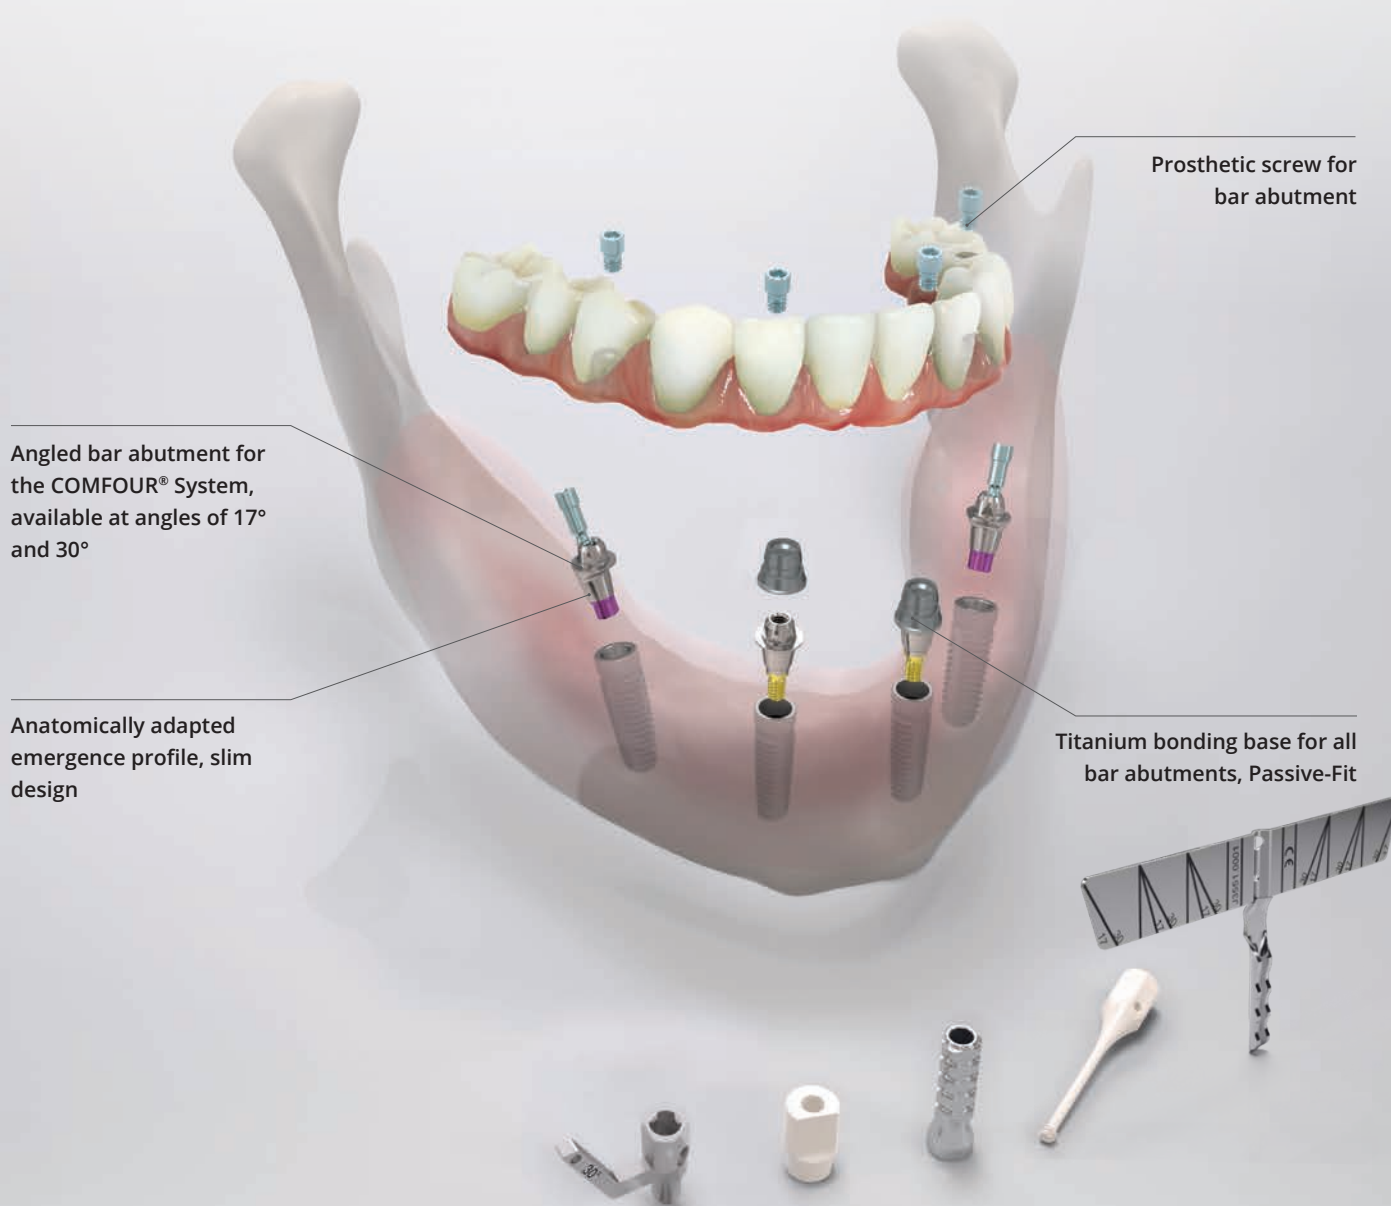
A special CONELOG® Disconnecter is available for the easy removal of CONELOG® Abutments from CONELOG® Implants or lab analogs. First the CONELOG® Abutment screw/ or lab screw is removed and the disconnecter is screwed into the screw canal until the abutment releases from the internal cone of the CONELOG® Implant or lab implant.



COMFOUR® System

Occlusally screw-retained restorations are state-of-the-art. With the COMFOUR® System, edentulous patients are given the option of immediate, comfortable and permanent dentures on four or six implants as a rule – and thus a considerable gain in quality of life. But clinicians too can look forward to considerably greater comfort and freedom. COMFOUR® offers several treatment concepts. In addition to occlusally screw-retained crowns and bridges for immediate and delayed restorations, the multi-optional system also permits bar restorations on straight and angled bar abutments.

COMFOUR® offers a wide range of options to master the challenges in practice routine easier and with less time in future. Next to its versatility, the COMFOUR® Prosthetic system excels through its slim design in particular. All components are of delicate and low design, which simplifies prosthetic restorations considerably for dentists and dental technicians. In addition, a number of technical highlights ensure that COMFOUR® is not simply just a name, but also a program – for users and patients alike.



COMFOUR® offers a large selection of options to manage the requirements of your practice. Easier and more time-saving.

Digital service

Individually CAD/CAM fabricated prosthetics, scanning and design services, 3D implant planning, printed drilling templates and jaw models are available from Camlog through our DEDICAM® Service Division. Personal support with the accustomed competence of our employees as well as processes optimized right down to the finest detail ensure a high degree of certainty of results with the greatest possible individual freedom. Extensive libraries for the open CAD systems from 3Shape, exocad and Dental Wings are available for implant-supported restorations. Discover your options and start your digital future with DEDICAM®.


DEDICAM® Services are not available in all countries. Please ask your local Camlog representative for details.



DEDICAM®

DIGITAL CONCEPTS

Color-coding of the surgical and prosthetical CONELOG® Products



3.3 mm 3.8 mm 4.3 mm 5.0 mm

Explanation of symbols

	CE-label
	Consult instructions for use
	Caution, observe the warning notices
	Medical device
	Article number
	Lot number
	Sterilized using irradiation
	Single sterile barrier system with protective packaging outside
	Non-sterile
	Date of manufacture
	Use-by date
	Do not resterilize
	Do not reuse
	Do not use if package is damaged
	Keep away from sunlight
	Temperature limit
	Manufacturer
	MR-Conditional
	Caution: US Federal law restricts this device to sale by or on the order of a dentist or physician.

Explanation of abbreviations

Ø	Diameter
AØ	Apical diameter
GØ	Gingival diameter
PPØ	Prosthetic platform diameter
L	Length
GH	Gingival height
PEEK	Poly ether ether ketone
POM	Polyoxymethylene
PPSU	Polyphenylsulfone

General safety instructions and warnings

The descriptions in this product catalog are not sufficient to allow immediate use of the CONELOG® Implant System. Instruction by a surgeon experienced in using the CONELOG® Implant System is strongly recommended.

Packaging PROGRESSIVE-LINE Implants

Secondary packaging

Sealed, folding box with color-coded product label

Inner Implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer Implant packaging



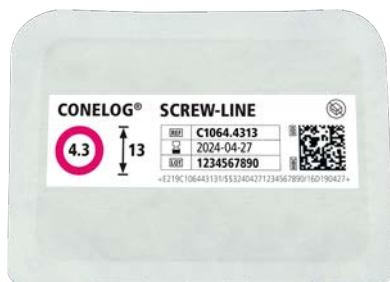
Packaging SCREW-LINE Implants

Secondary packaging

Sealed, folding box with color-coded product label

Inner Implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer Implant packaging







Planning

X-Ray Planning foils and X-Ray Transfer pictures

	Article	Art. No.	Ø
	X-Ray Planning foil 1.25:1 CONELOG® PROGRESSIVE-LINE Implants Magnification 25%	C5300.9014	-
	X-Ray Planning foil 1.25:1 CONELOG® SCREW-LINE Implants Magnification 25%	C5300.9010	-
	X-Ray Planning foil 1.4:1 CONELOG® PROGRESSIVE-LINE Implants Magnification 40%	C5300.9015	-
	X-Ray Planning foil 1.4:1 CONELOG® SCREW-LINE Implants Magnification 40%	C5300.9011	-
	X-Ray Transfer pictures 1.25:1 CONELOG® SCREW-LINE Implants Planning slide, self-adhesive Magnification 25%	C5300.9080	3.3 mm
		C5300.9081	3.8 mm
		C5300.9082	4.3 mm
		C5300.9083	5.0 mm

CT-Planning

for 3-D X-Ray Planning and drilling template

	Article	Art. No.	L
	CT-tube for drill Ø 2.0 mm*, corrugated tubing pack of 10 internal diameter 2.1 mm external diameter 2.5 mm Material Titanium alloy	A2002.2000	4.0 mm 10.0 mm
	CT-tube for drill Ø 2.2 mm, corrugated tubing pack of 10 internal diameter 2.3 mm external diameter 2.7 mm Material Titanium alloy	A2222.2200	4.0 mm 10.0 mm
	Drill for CT-tube (for A2002.2000) Ø 2.6 mm Material Stainless steel	A2050.2600	-
	Drill for CT-tube (for A2222.2200) Ø 2.8 mm Material Stainless steel	A2050.2800	-

* for pilot drills J5051.2003 and pilot drills SCREW-LINE J5051.2000



PROGRESSIVE-LINE

Implants with snap-in insertion post

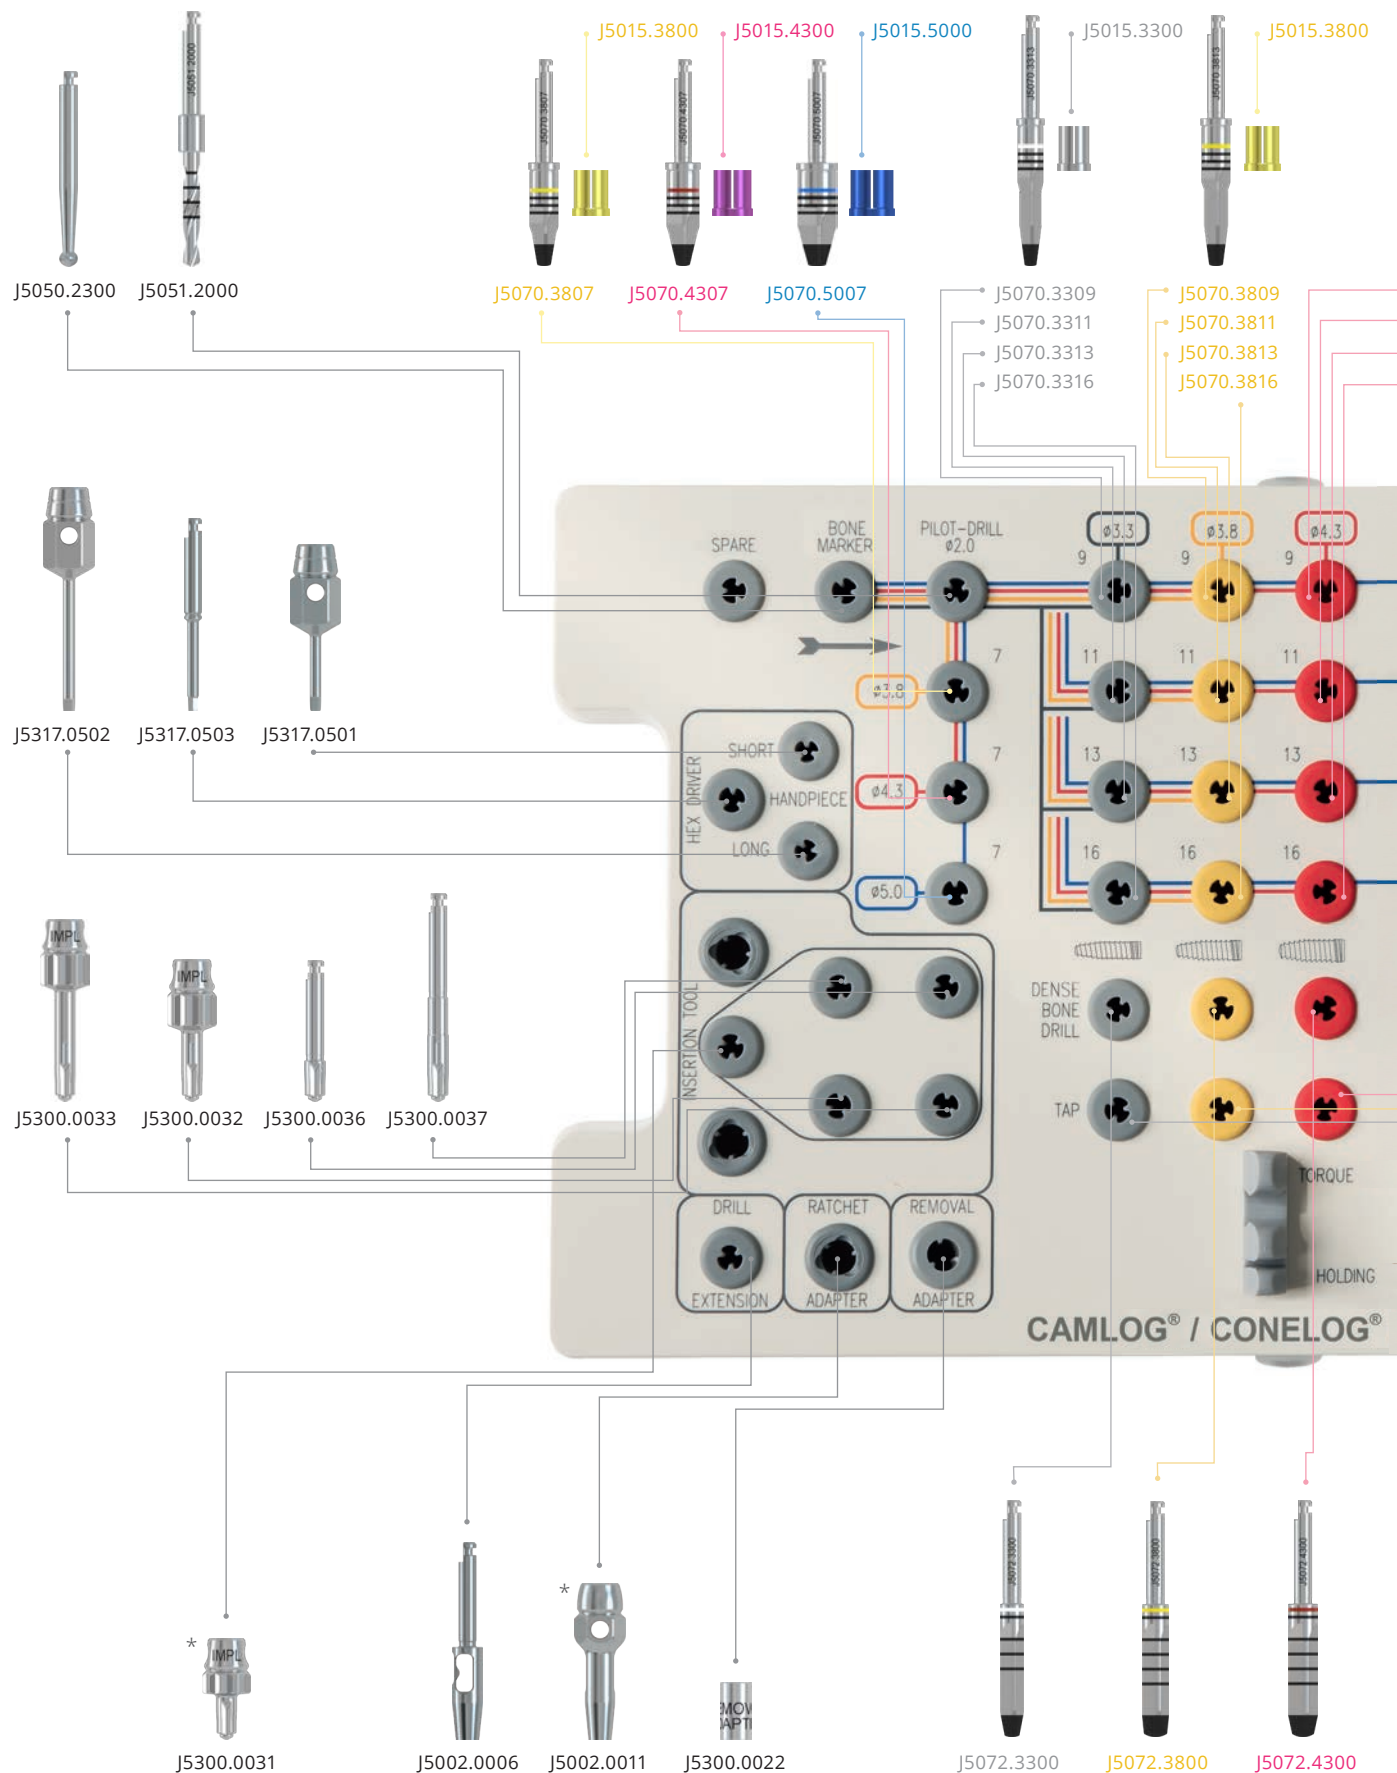
	Article	Art. No.	Ø	L	A Ø
	CONELOG® PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1086.3309	3.3 mm	9 mm	2.2 mm
		C1086.3311		11 mm	
		C1086.3313		13 mm	
		C1086.3316		16 mm	
		C1086.3807	3.8 mm	7 mm	3.0 mm
		C1086.3809		9 mm	
		C1086.3811		11 mm	2.7 mm
		C1086.3813		13 mm	
		C1086.3816		16 mm	
		C1086.4307	4.3 mm	7 mm	3.0 mm
		C1086.4309		9 mm	
		C1086.4311		11 mm	2.7 mm
		C1086.4313		13 mm	
		C1086.4316		16 mm	
		C1086.5007	5.0 mm	7 mm	3.5 mm
		C1086.5009		9 mm	
		C1086.5011		11 mm	3.2 mm
		C1086.5013		13 mm	
		C1086.5016		16 mm	

Implants with screw-mounted insertion post

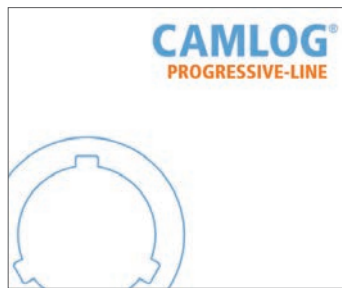
	Article	Art. No.	Ø	L	A Ø
	CONELOG® PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1085.3309	3.3 mm	9 mm	2.2 mm
		C1085.3311		11 mm	
		C1085.3313		13 mm	
		C1085.3316		16 mm	
		C1085.3807	3.8 mm	7 mm	3.0 mm
		C1085.3809		9 mm	
		C1085.3811		11 mm	2.7 mm
		C1085.3813		13 mm	
		C1085.3816		16 mm	
		C1085.4307	4.3 mm	7 mm	3.0 mm
		C1085.4309		9 mm	
		C1085.4311		11 mm	2.7 mm
		C1085.4313		13 mm	
		C1085.4316		16 mm	
		C1085.5007	5.0 mm	7 mm	3.5 mm
		C1085.5009		9 mm	
		C1085.5011		11 mm	3.2 mm
		C1085.5013		13 mm	
		C1085.5016		16 mm	

PROGRESSIVE-LINE

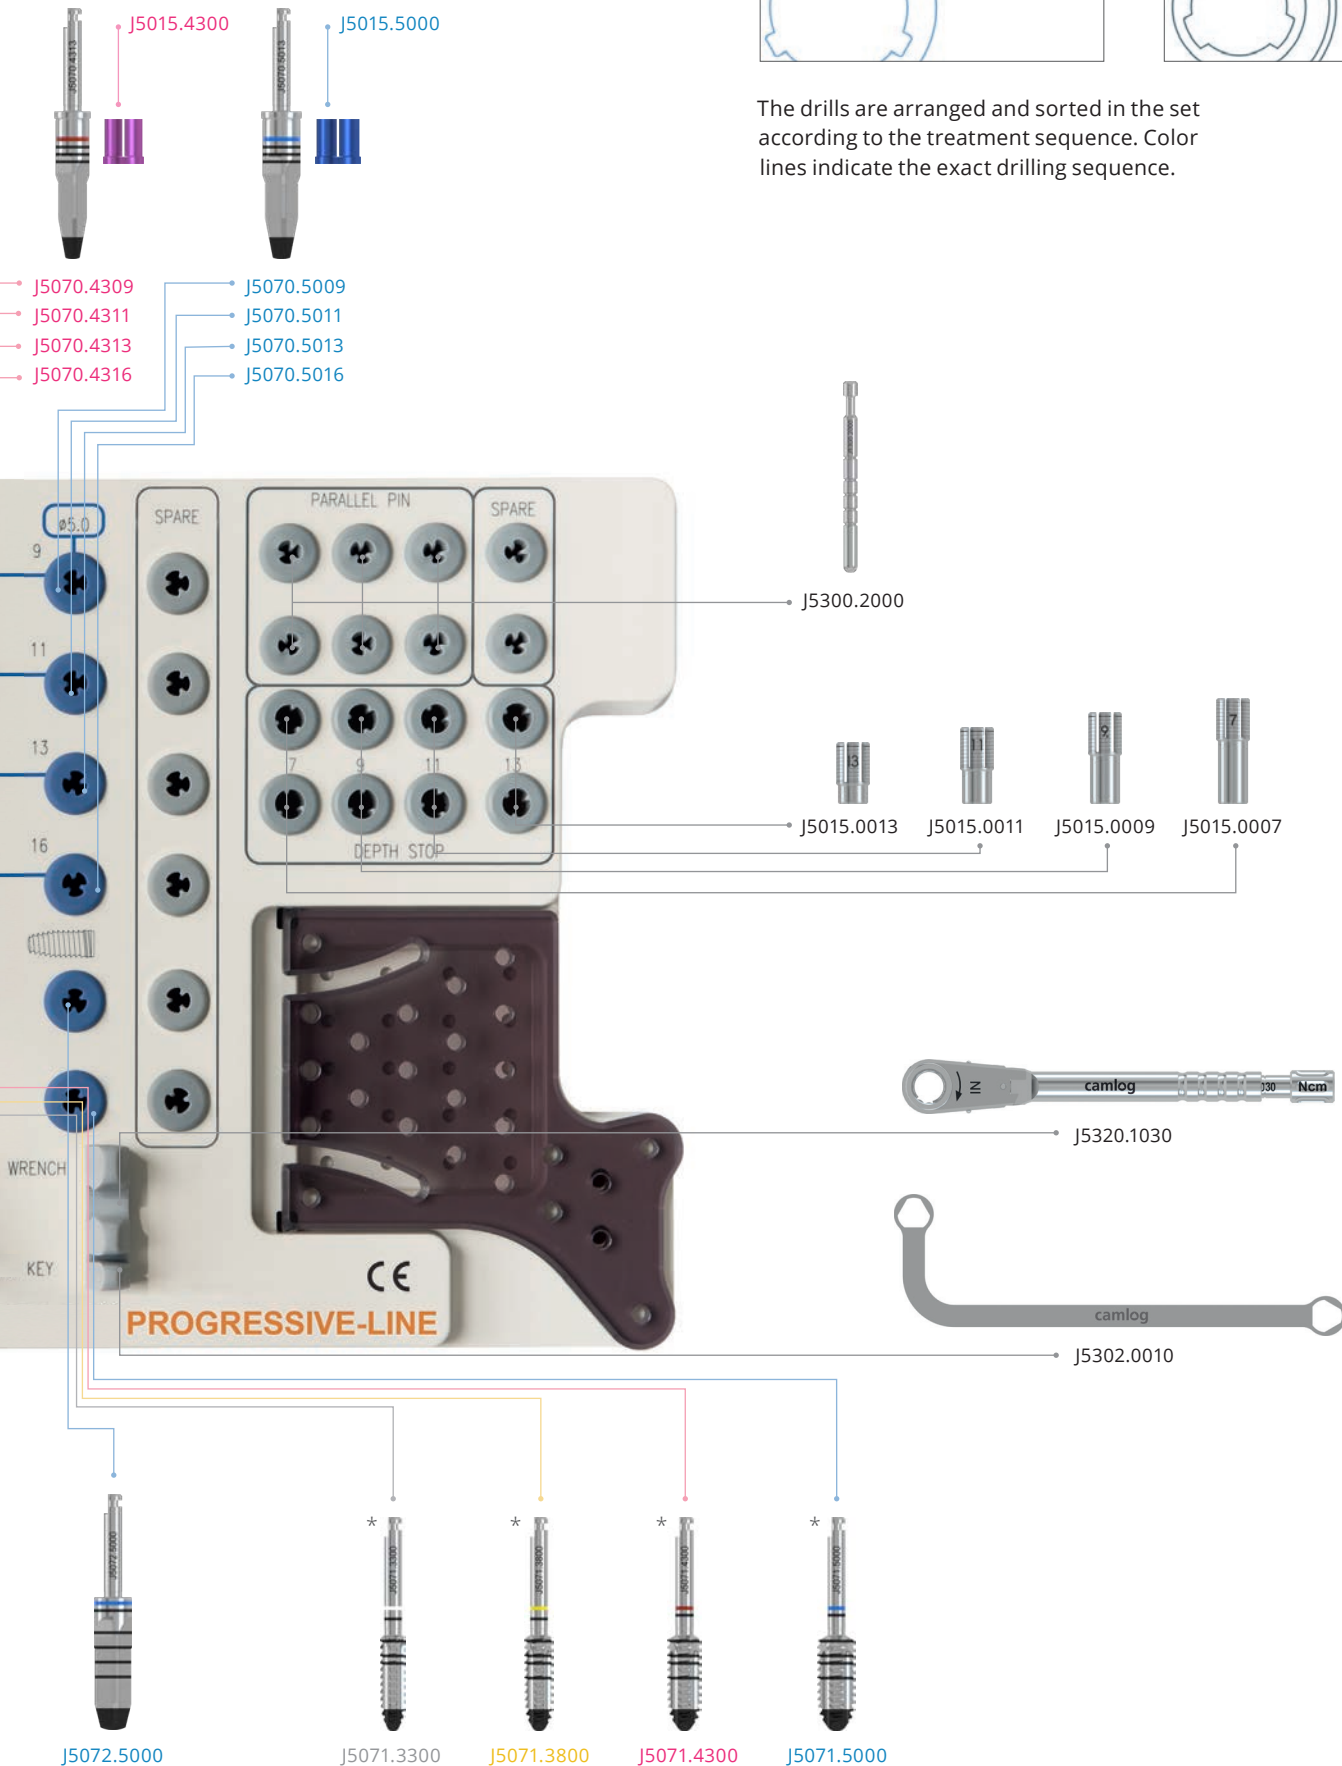
Surgery set CAMLOG®/CONELOG®



* These articles are not included in the surgery set and must be ordered separately.

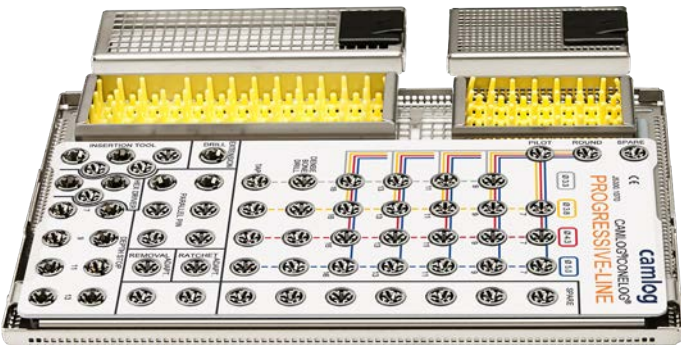
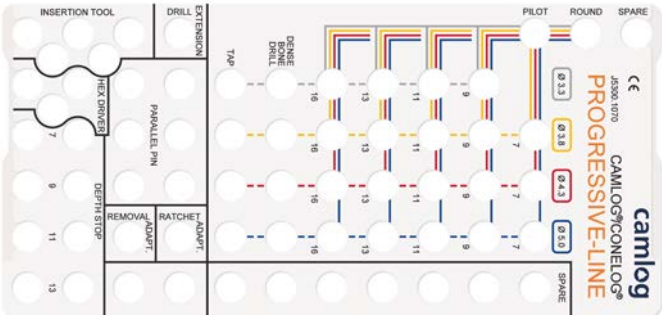


The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.



PROGRESSIVE-LINE

Surgery set

	Article	Art. No.
 A white plastic tray containing a variety of surgical instruments. The instruments are organized into sections: 'REMOVAL TOOL' (left), 'TAP' (center), and 'HOLDING KEY' (right). The instruments are color-coded (yellow, red, blue, black) and labeled with numbers. A torque wrench and a holding key are also visible.	Surgery set CAMLOG®/CONELOG® PROGRESSIVE-LINE contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post (taps are not included)	J5300.0065
 An empty white plastic tray, identical in design to the one above, showing the layout of the instrument compartments and the 'HOLDING KEY' section.	Surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content	J5300.8917
 A white plastic tray with two yellow instrument holders at the top. The main section contains a grid of circular holes for instruments, labeled with numbers and names like 'INSERTION TOOL', 'DRILL', 'TAP', 'REMOVAL', 'RATCHET', 'ADAPT.', 'PILOT', 'ROUND', and 'SPARE'. A pattern is visible on the right side.	Surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE incl. pattern, without content	J5300.8970
 A white plastic pattern for the surgery wash tray. It features a grid of circular holes, labeled with numbers and names like 'INSERTION TOOL', 'DRILL', 'TAP', 'REMOVAL', 'RATCHET', 'ADAPT.', 'PILOT', 'ROUND', and 'SPARE'. The pattern is designed to fit into the wash tray.	Pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE Material PPSU	J5300.1070

Preparation of the implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

Surgical instruments

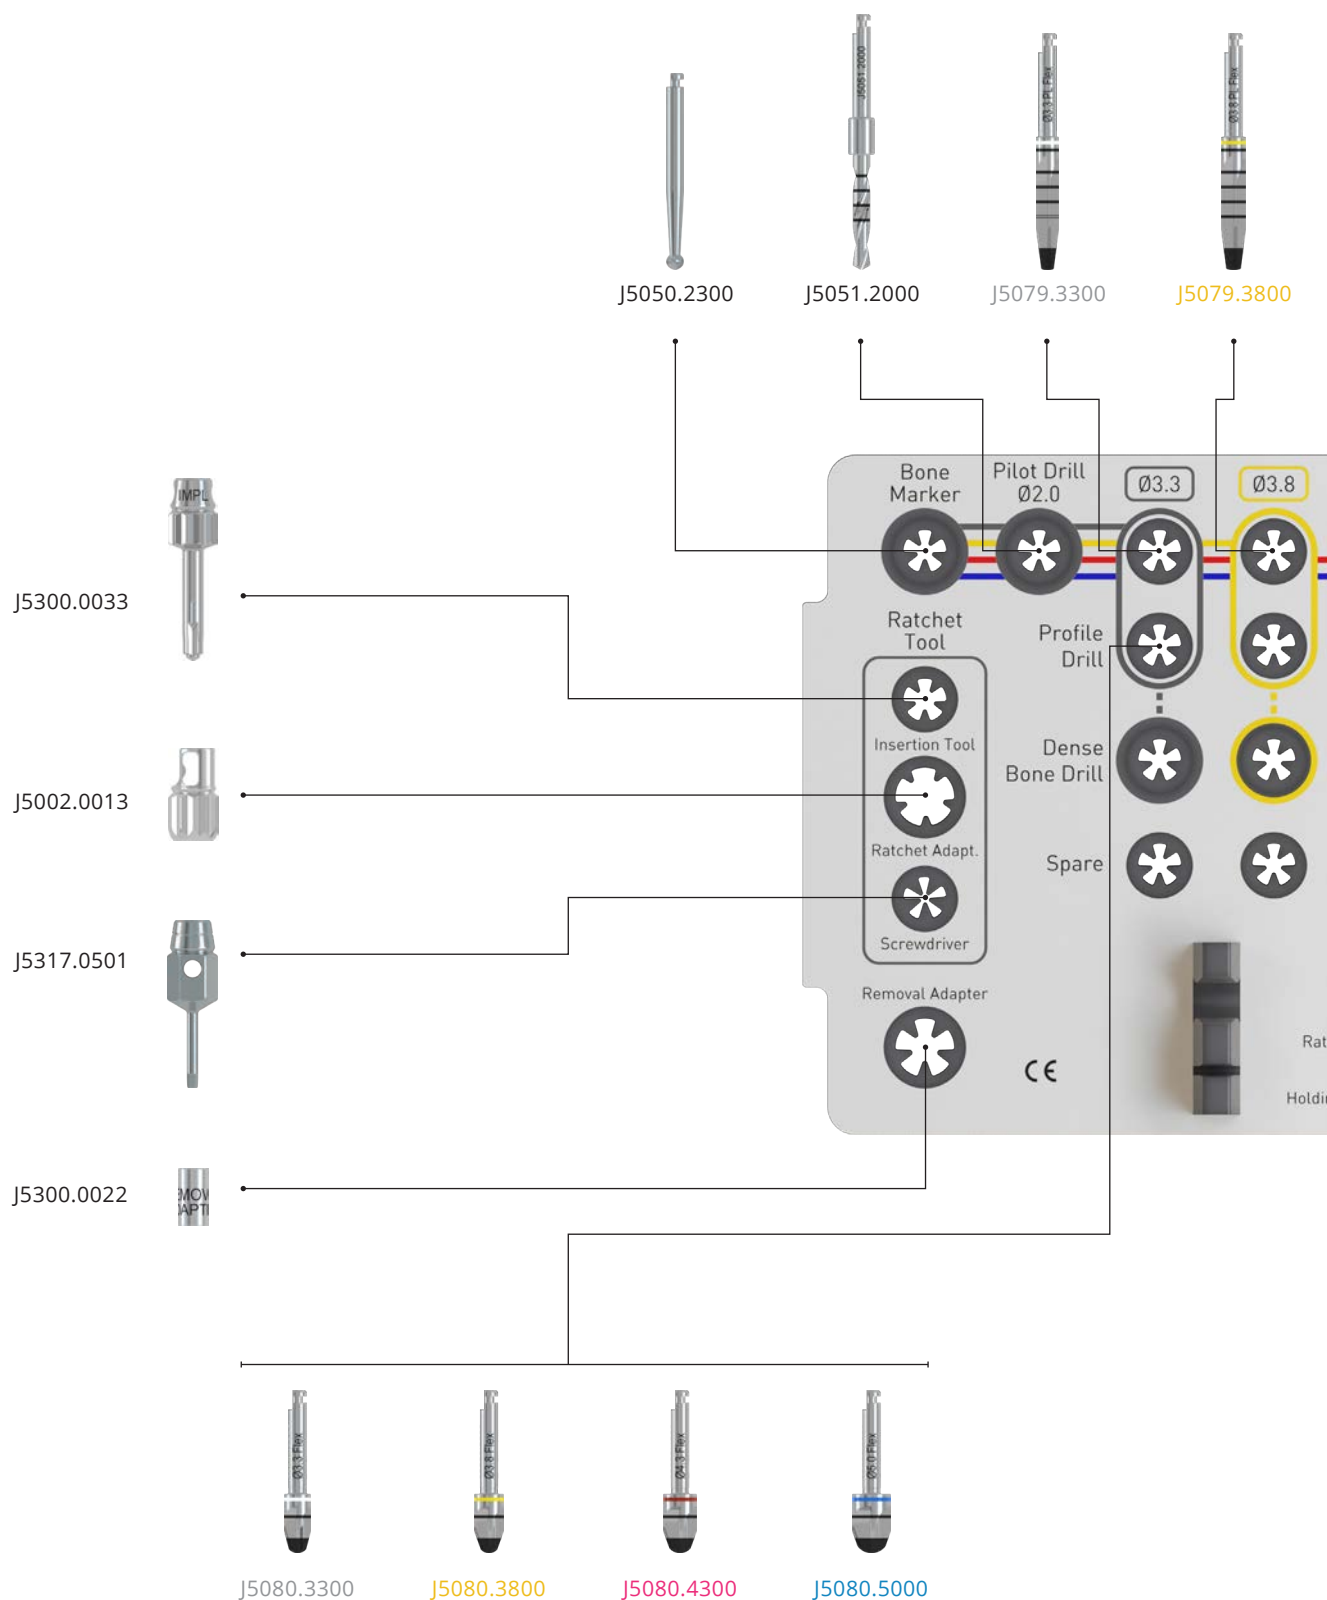
	Article	Art. No.	Ø	L
	Form drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5070.3309	3.3 mm	9 mm
		J5070.3311		11 mm
		J5070.3313		13 mm
		J5070.3316		16 mm
		J5070.3807	3.8 mm	7 mm
		J5070.3809		9 mm
		J5070.3811		11 mm
		J5070.3813		13 mm
		J5070.3816		16 mm
		J5070.4307	4.3 mm	7 mm
		J5070.4309		9 mm
		J5070.4311		11 mm
		J5070.4313		13 mm
		J5070.4316		16 mm
		J5070.5007	5.0 mm	7 mm
		J5070.5009		9 mm
		J5070.5011		11 mm
		J5070.5013		13 mm
		J5070.5016		16 mm
	Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	Dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	
		J5072.4300	4.3 mm	
		J5072.5000	5.0 mm	
	Tap PROGRESSIVE-LINE resterilizable Material Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	
		J5071.4300	4.3 mm	
		J5071.5000	5.0 mm	
	Removal adapter for CAMLOG® and CONELOG® suitable for all implant diameters Material Stainless steel	J5300.0022*	3.3 mm	6.2 mm
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Paralleling pin PROGRESSIVE-LINE with depth marks (for pilot drilling Ø 2.0 mm) Material Titanium alloy	J5300.2000	-	-

* only for use with PROGRESSIVE-LINE Implants with snap-in insertion post

PROGRESSIVE-LINE Flex

Surgery set CAMLOG®/CONELOG®

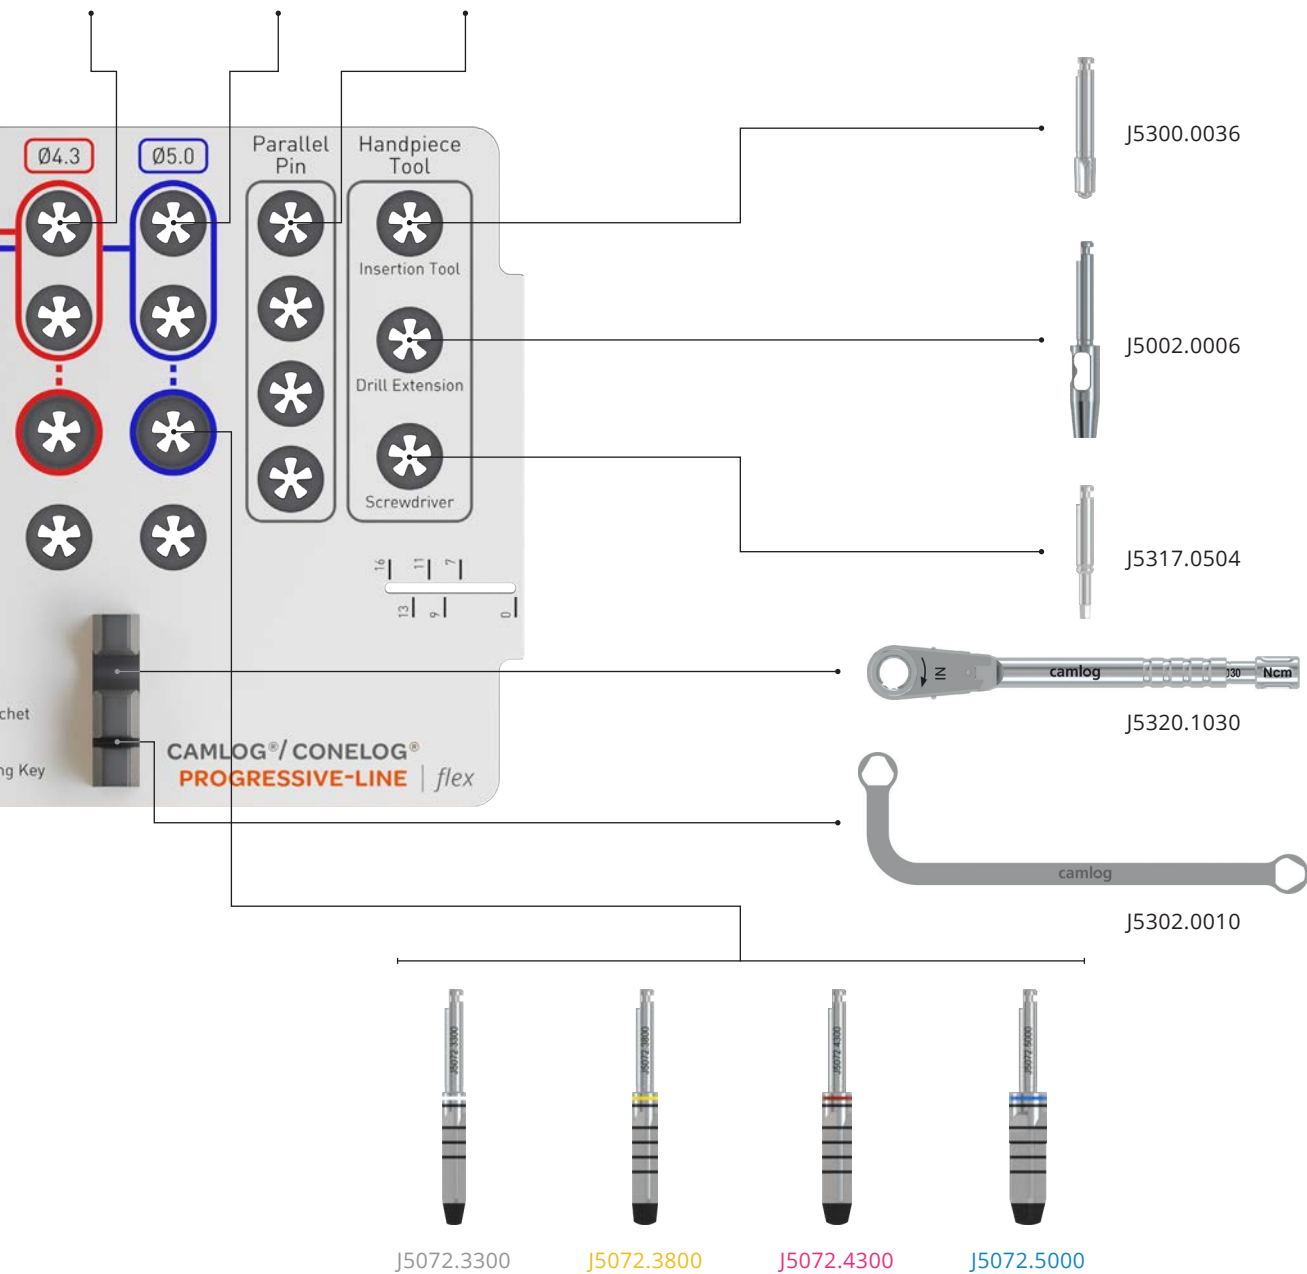
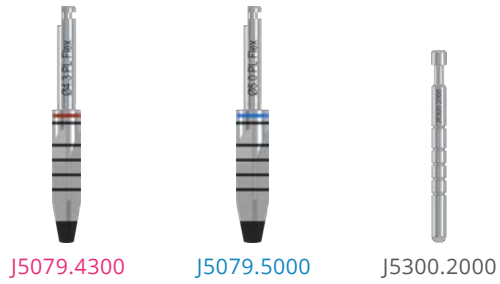
NEW



* Optional articles, can be purchased separately



The drills are arranged and sorted in the set according to the treatment sequence. Color lines indicate the exact drilling sequence.



PROGRESSIVE-LINE Flex

Surgery set

	Article	Art. No.
 A photograph of the CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex Surgery set. The set is a white, rectangular case with a handle. It contains various surgical instruments, including a torque wrench, a holding key, and several drill bits, all organized in a grid-like layout. The instruments are color-coded and labeled with their respective functions and sizes.	Surgery set CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post	J5300.0071
 A photograph of the CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex Surgery tray. The tray is a white, rectangular case with a handle. It contains various surgical instruments, including a torque wrench, a holding key, and several drill bits, all organized in a grid-like layout. The instruments are color-coded and labeled with their respective functions and sizes.	Surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex without content	J5300.8920

Surgical instruments

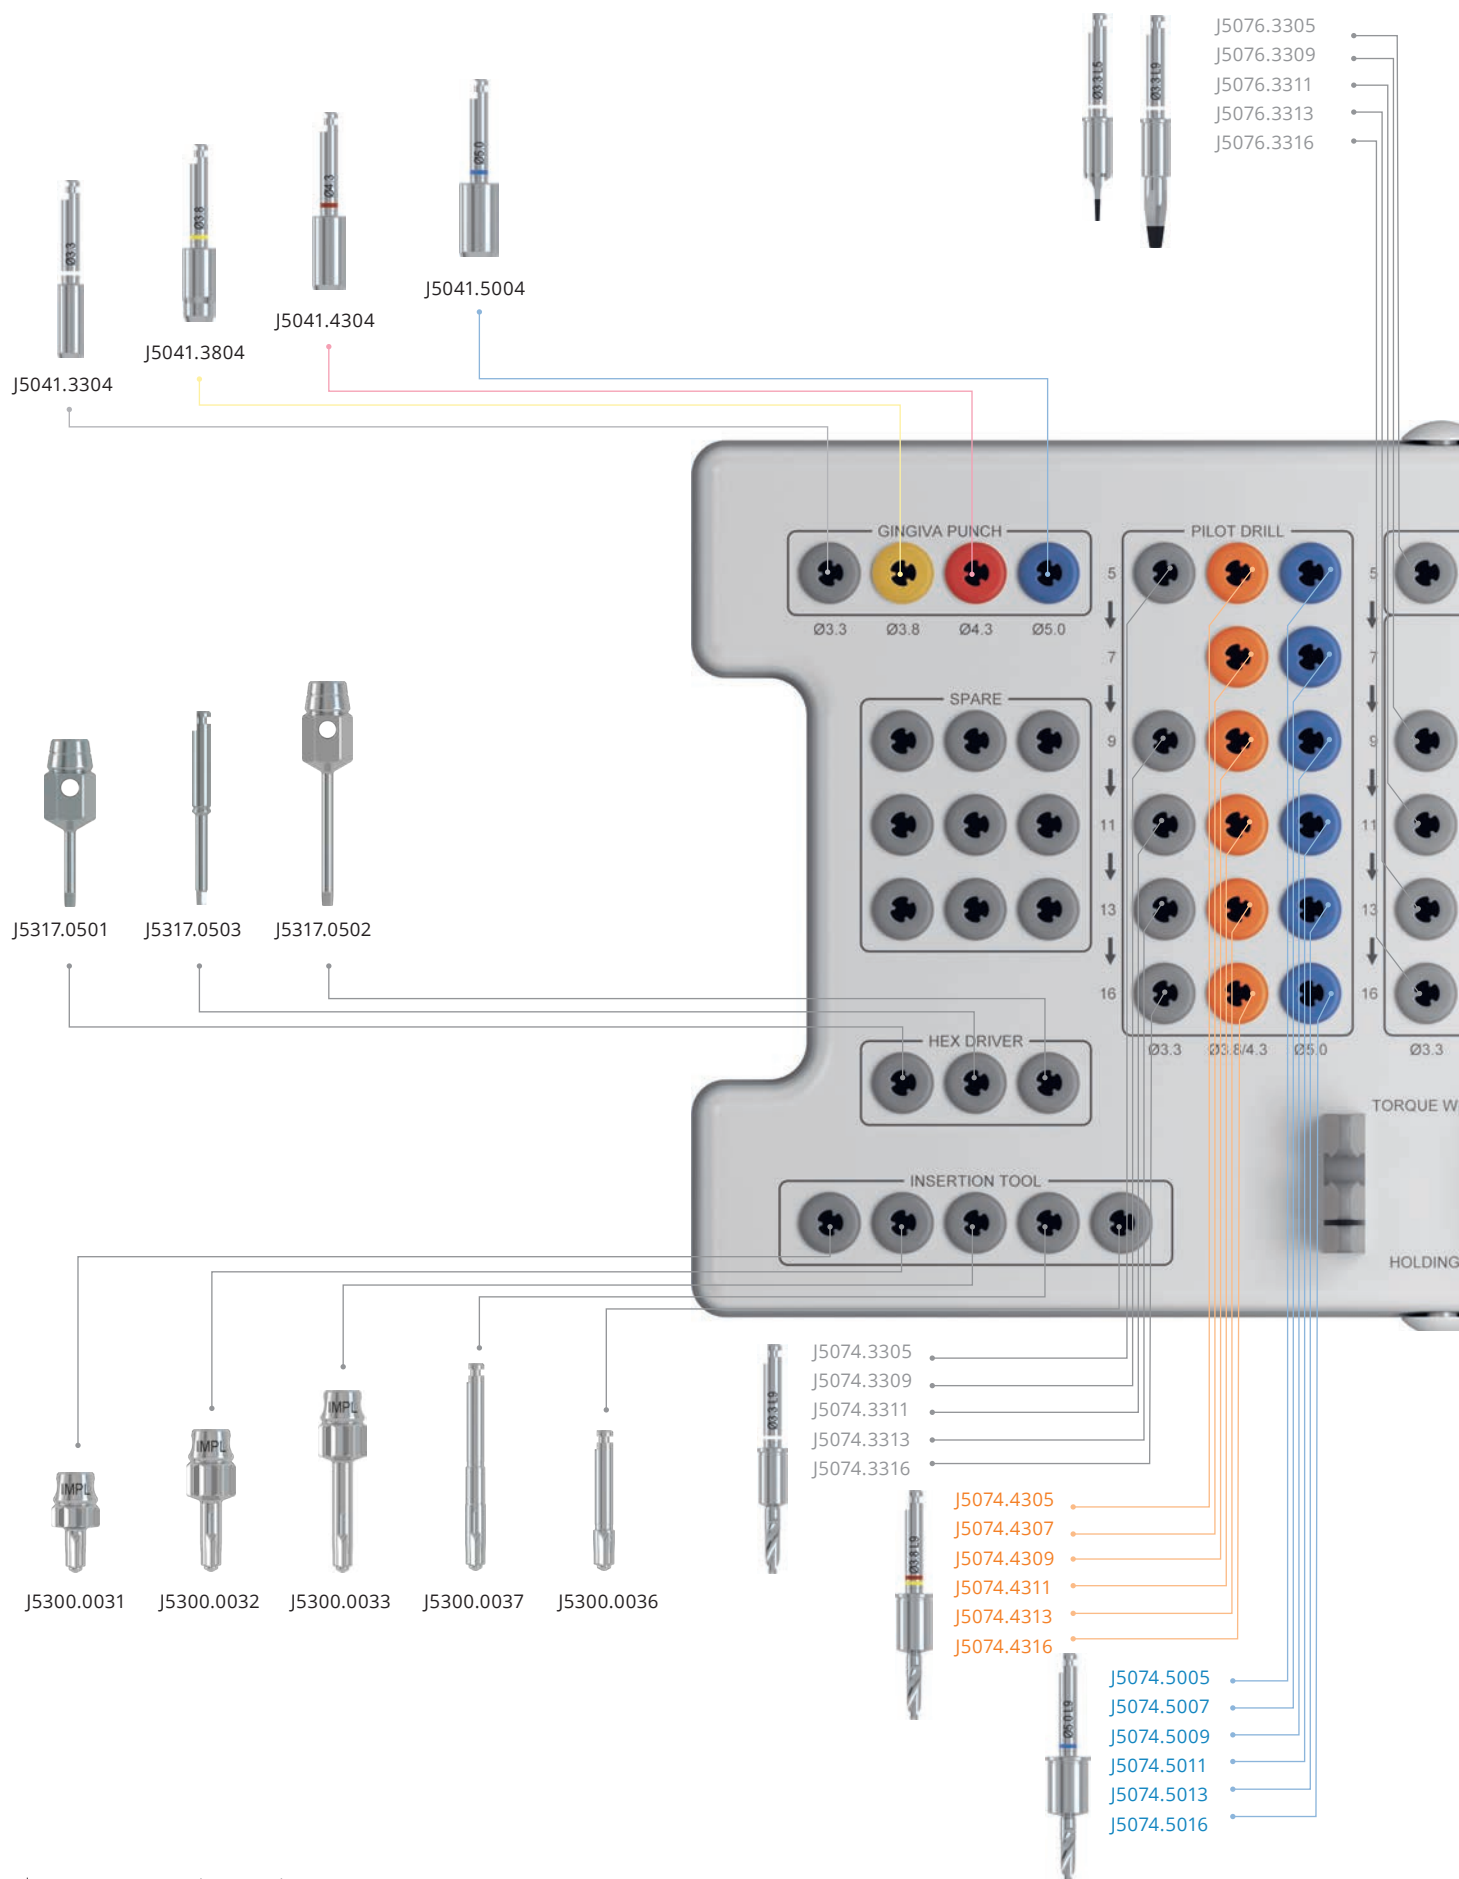
	Article	Art. No.	Ø	L
	Drill PROGRESSIVE-LINE Flex resterilizable Material Stainless steel	J5079.3300	3.3 mm	-
		J5079.3800	3.8 mm	
		J5079.4300	4.3 mm	
		J5079.5000	5.0 mm	
	Profile drill PROGRESSIVE-LINE Flex resterilizable Material Stainless steel	J5080.3300	3.3 mm	-
		J5080.3800	3.8 mm	
		J5080.4300	4.3 mm	
		J5080.5000	5.0 mm	
	Wrench adapter Material Stainless steel	J5002.0013	-	11 mm

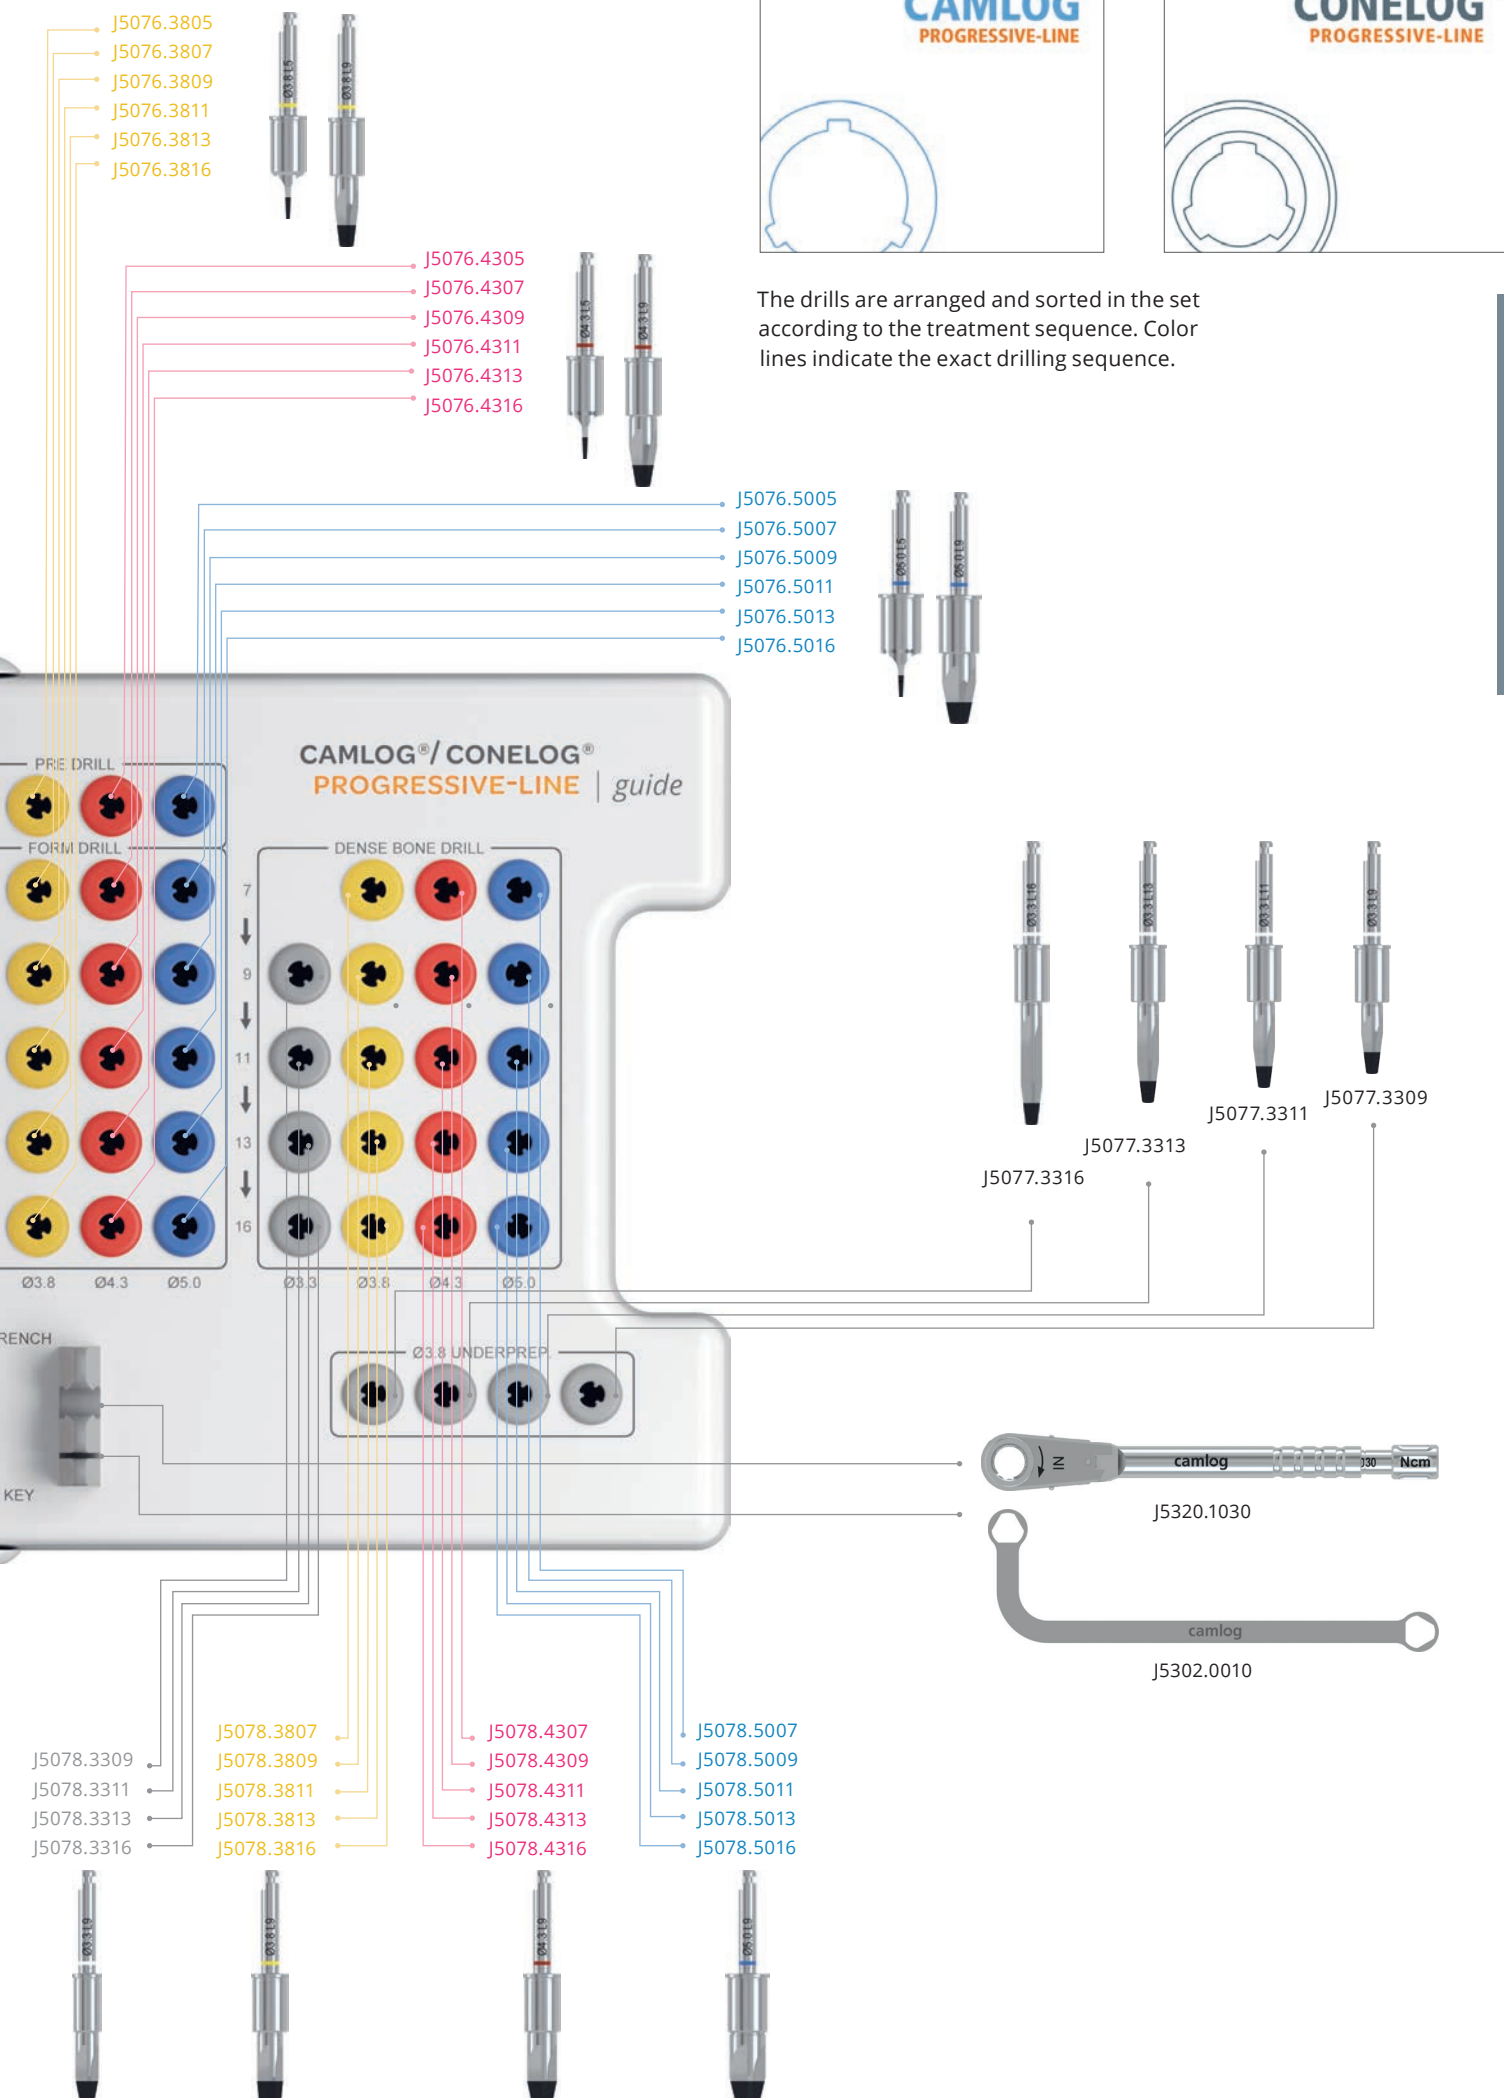
Preparation of the implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

PROGRESSIVE-LINE

Guide System Surgery set CAMLOG®/CONELOG®

NEW





PROGRESSIVE-LINE

Guide System

	Article	Art. No.
	Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content	J5300.8919

	Article	Art. No.	Ø	L
	Guide System gingiva punch PROGRESSIVE-LINE resterilizable Material Stainless steel	J5041.3304	3.3 mm	-
		J5041.3804	3.8 mm	
		J5041.4304	4.3 mm	
		J5041.5004*	5.0 mm	
	Guide System pilot drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5074.3305	3.3 mm	5 mm
		J5074.3309		9 mm
		J5074.3311		11 mm
		J5074.3313		13 mm
		J5074.3316		16 mm
		J5074.4305	3.8 mm	5 mm
		J5074.4307		7 mm
		J5074.4309		9 mm
		J5074.4311		11 mm
		J5074.4313	4.3 mm	13 mm
		J5074.4316		16 mm
		J5074.5005*		5 mm
		J5074.5007*	5.0 mm	7 mm
		J5074.5009*		9 mm
		J5074.5011*		11 mm
		J5074.5013*		13 mm
		J5074.5016*		16 mm

* product availability expected for end of Q1/2021

Notes


CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1085.xxxx with screw-mounted insertion post can be used with the PROGRESSIVE-LINE Guide System.

	Article	Art. No.	Ø	L
	Guide System pre-drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5076.3305	3.3 mm	5 mm
		J5076.3805	3.8 mm	
		J5076.4305	4.3 mm	
		J5076.5005*	5.0 mm	
	Guide System form drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5076.3309	3.3 mm	9 mm
		J5076.3311		11 mm
		J5076.3313		13 mm
		J5076.3316		16 mm
		J5076.3807	3.8 mm	7 mm
		J5076.3809		9 mm
		J5076.3811		11 mm
		J5076.3813		13 mm
		J5076.3816		16 mm
		J5076.4307	4.3 mm	7 mm
		J5076.4309		9 mm
		J5076.4311		11 mm
		J5076.4313		13 mm
		J5076.4316		16 mm
		J5076.5007*	5.0 mm	7 mm
		J5076.5009*		9 mm
		J5076.5011*		11 mm
		J5076.5013*		13 mm
		J5076.5016*		16 mm
	Guide System dense bone drill PROGRESSIVE-LINE resterilizable Material Stainless steel	J5078.3309	3.3 mm	9 mm
		J5078.3311		11 mm
		J5078.3313		13 mm
		J5078.3316		16 mm
		J5078.3807	3.8 mm	7 mm
		J5078.3809		9 mm
		J5078.3811		11 mm
		J5078.3813		13 mm
		J5078.3816		16 mm
		J5078.4307	4.3 mm	7 mm
		J5078.4309		9 mm
		J5078.4311		11 mm
		J5078.4313		13 mm
		J5078.4316		16 mm
		J5078.5007*	5.0 mm	7 mm
		J5078.5009*		9 mm
		J5078.5011*		11 mm
		J5078.5013*		13 mm
		J5078.5016*		16 mm
	Guide System form drill for Ø 3.8 mm under preparation PROGRESSIVE-LINE resterilizable Material Stainless steel	J5077.3309	3.3 mm	9 mm
		J5077.3311		11 mm
		J5077.3313		13 mm
		J5077.3316		16 mm

* product availability expected for end of Q1/2021

PROGRESSIVE-LINE

Guide System

	Article	Art. No.	Ø	L
	Guide System template drill PROGRESSIVE-LINE for Guide System guiding sleeve Material Stainless steel	J3753.3300	3.3 mm	-
		J3753.4300	3.8 mm 4.3 mm	
		J3753.5000*	5.0 mm	
	Guide System guiding sleeve PROGRESSIVE-LINE** (2 units) Material Titanium alloy	J3754.3301	3.3 mm	-
		J3754.3801	3.8 mm	
		J3754.4301	4.3 mm	
		J3754.5001*	5.0 mm	
	Guide System setting tool PROGRESSIVE-LINE for Guide System guiding sleeve Material Stainless steel	J3717.3300	3.3 mm	-
		J3717.4300	3.8 mm 4.3 mm	
		J3717.5000*	5.0 mm	
	Guide System check-up pin PROGRESSIVE-LINE for Guide System guiding sleeve Material Stainless steel	J5301.3310	3.3 mm	-
		J5301.4310	3.8 mm 4.3 mm	
		J5301.5010*	5.0 mm	
	Guide System CONELOG® Insertion post, screw-mounted for CONELOG® Lab implant/implant analog, incl. fixing screw (2 units) Material Titanium alloy	C2026.3303	3.3 mm	-
		C2026.3803	3.8 mm	
		C2026.4303	4.3 mm	
		C2026.5003*	5.0 mm	

* product availability expected for end of Q1/2021

** only for use with PROGRESSIVE-LINE Implants with screw-mounted insertion post

SCREW-LINE

Implants with snap-in insertion post

	Article	Art. No.	Ø	L	A Ø
	CONELOG® SCREW-LINE Implant, Promote® plus incl. snap-in insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1066.3309*	3.3 mm	9 mm	2.7 mm
		C1066.3311*		11 mm	
		C1066.3313*		13 mm	
		C1066.3316*		16 mm	
		C1066.3807*	3.8 mm	7 mm	3.5 mm
		C1066.3809*		9 mm	
		C1066.3811*		11 mm	
		C1066.3813*		13 mm	
		C1066.3816*		16 mm	
		C1066.4307*	4.3 mm	7 mm	3.9 mm
		C1066.4309*		9 mm	
		C1066.4311*		11 mm	
		C1066.4313*		13 mm	
		C1066.4316*		16 mm	
		C1066.5007*	5.0 mm	7 mm	4.6 mm
		C1066.5009*		9 mm	
		C1066.5011*		11 mm	
		C1066.5013*		13 mm	
		C1066.5016*		16 mm	

* Please note: CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1066.xxxx succeed Implants with Art. No. C1064.xxxx starting in October 2020. Depending on your country CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1064.xxxx might still be available for a longer period.

Implants with screw-mounted insertion post

	Article	Art. No.	Ø	L	A Ø
	CONELOG® SCREW-LINE Implant, Promote® plus incl. screw-mounted insertion post and cover screw, sterile Material Titanium Grade 4 US Pat. No. 9,545,293	C1065.3309**	3.3 mm	9 mm	2.7 mm
		C1065.3311**		11 mm	
		C1065.3313**		13 mm	
		C1065.3316**		16 mm	
		C1065.3807**	3.8 mm	7 mm	3.5 mm
		C1065.3809**		9 mm	
		C1065.3811**		11 mm	
		C1065.3813**		13 mm	
		C1065.3816**		16 mm	
		C1065.4307**	4.3 mm	7 mm	3.9 mm
		C1065.4309**		9 mm	
		C1065.4311**		11 mm	
		C1065.4313**		13 mm	
		C1065.4316**		16 mm	
		C1065.5007**	5.0 mm	7 mm	4.6 mm
		C1065.5009**		9 mm	
		C1065.5011**		11 mm	
		C1065.5013**		13 mm	
		C1065.5016**		16 mm	

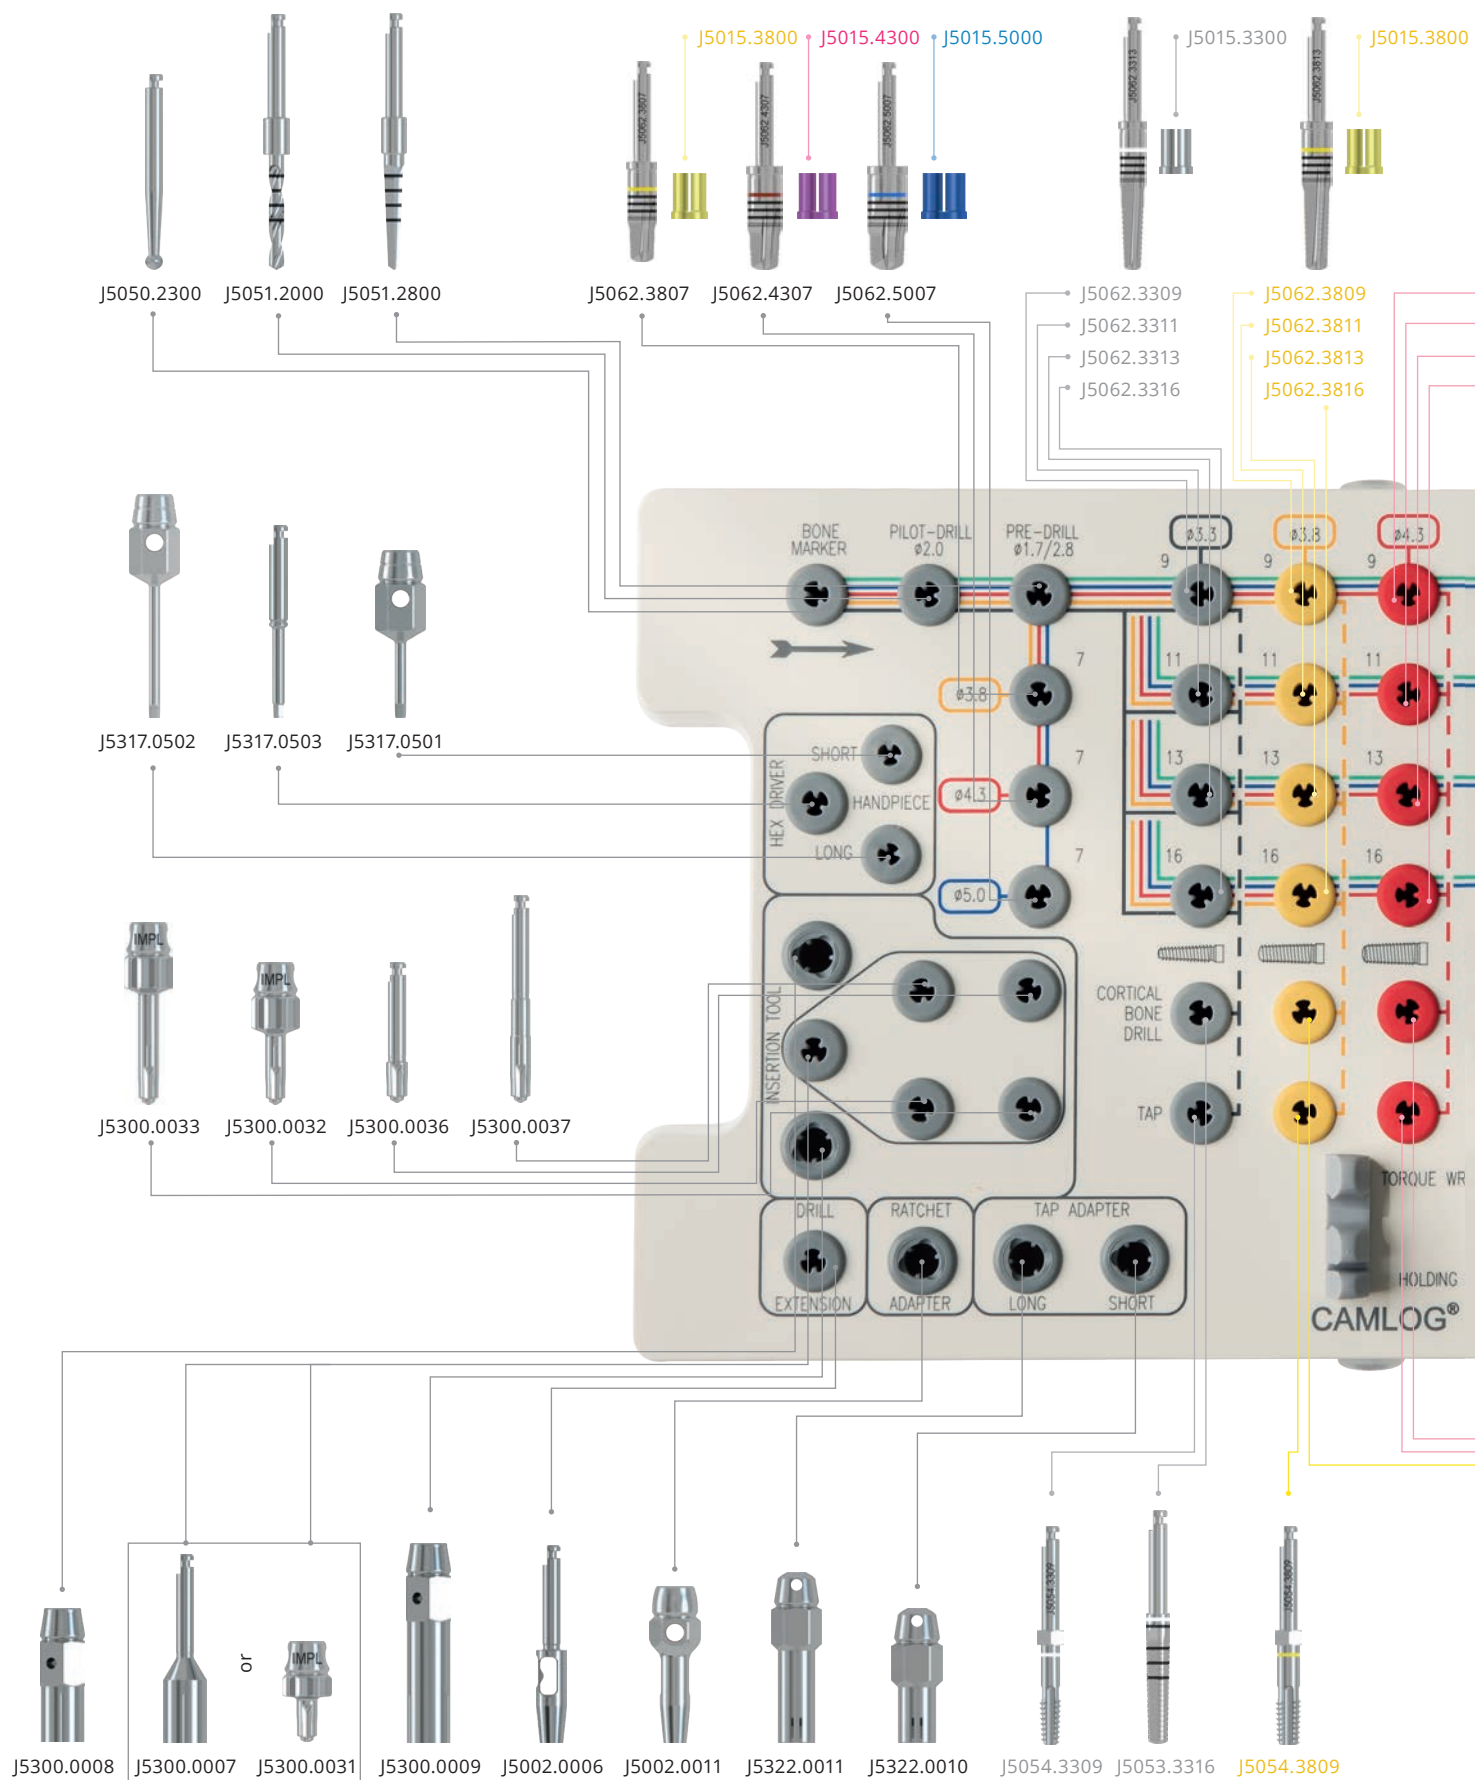
** Please note: CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1065.xxxx succeed Implants with Art. No. C1063.xxxx starting in October 2020. Depending on your country CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1063.xxxx might still be available for a longer period.

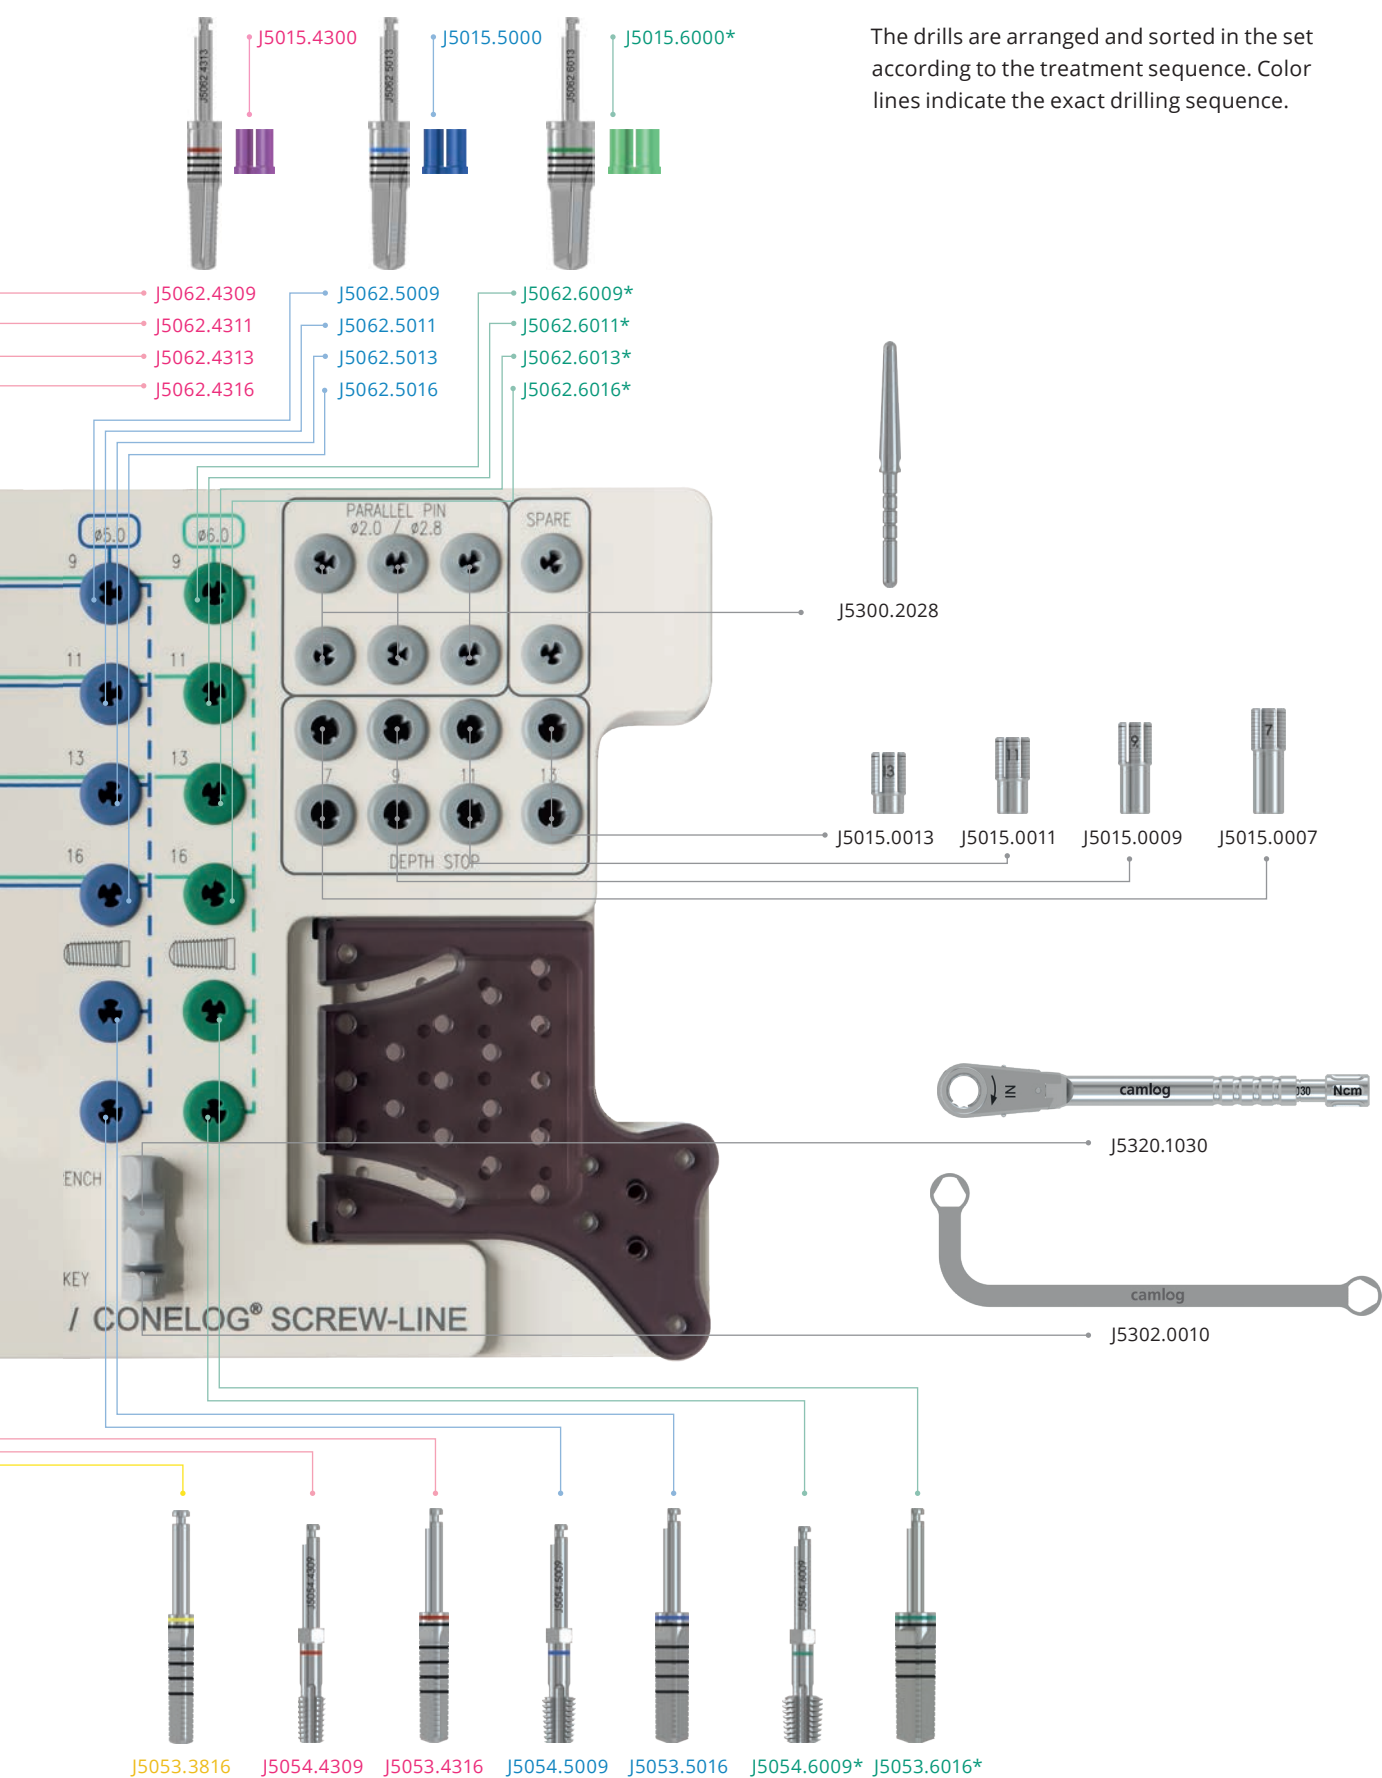
Notes

CONELOG® SCREW-LINE Implants Promote® plus with Art. No. C1064.xxxx and Art. No. C1065.xxxx can be used exclusively with the drivers Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034, J5300.0035, J5300.0036 or J5300.0037.

SCREW-LINE

Surgery set CAMLOG®/CONELOG®

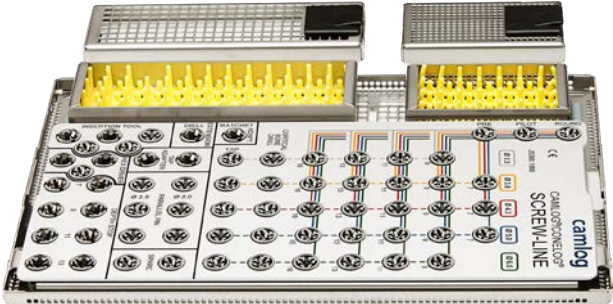
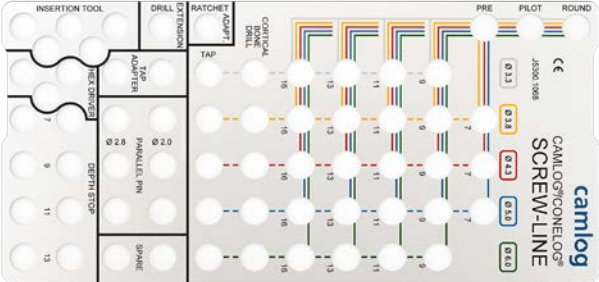




* only for CAMLOG® SCREW-LINE Implants $\varnothing 6.0$ mm

SCREW-LINE

Surgery set

	Article	Art. No.
	Surgery set CAMLOG®/CONELOG® SCREW-LINE contains all necessary surgical instruments sorted by color code, incl. torque wrench and holding key for insertion post (drills and taps for Ø 6.0 mm are not included)	J5300.0063
	Surgery tray CAMLOG®/CONELOG® SCREW-LINE without content	J5300.8916
	Surgery wash tray CAMLOG®/CONELOG® SCREW-LINE incl. pattern, without content	J5300.8968
	Pattern for surgery wash tray CAMLOG®/CONELOG® SCREW-LINE Material Aluminum	J5300.1068

Preparation of the implant bed for CAMLOG® SCREW-LINE Implants and for CONELOG® SCREW-LINE Implants is performed with identical instruments.

Surgical instruments

	Article	Art. No.	Ø	L
	Form drill SCREW-LINE resterilizable Material Stainless steel	J5062.3309	3.3 mm	9 mm
		J5062.3311		11 mm
		J5062.3313		13 mm
		J5062.3316		16 mm
		J5062.3807	3.8 mm	7 mm
		J5062.3809		9 mm
		J5062.3811		11 mm
		J5062.3813		13 mm
		J5062.3816		16 mm
		J5062.4307	4.3 mm	7 mm
		J5062.4309		9 mm
		J5062.4311		11 mm
		J5062.4313		13 mm
		J5062.4316		16 mm
		J5062.5007	5.0 mm	7 mm
		J5062.5009		9 mm
		J5062.5011		11 mm
		J5062.5013		13 mm
		J5062.5016		16 mm
	Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE resterilizable Material Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	Form drill SCREW-LINE Cortical bone resterilizable Material Stainless steel	J5053.3316	3.3 mm	-
		J5053.3816	3.8 mm	
		J5053.4316	4.3 mm	
		J5053.5016	5.0 mm	
	Tap SCREW-LINE with hexagon, resterilizable Material Stainless steel	J5054.3309	3.3 mm	-
		J5054.3809	3.8 mm	
		J5054.4309	4.3 mm	
		J5054.5009	5.0 mm	

SCREW-LINE

Guide System

	Article	Art. No.	Ø	L
	Guide System pilot drill set internal irrigation, sterile (for pilot drills Ø 2.0 mm) Material Stainless steel	J5063.3309	3.3 mm	9 mm (incl. 5 mm)**
		J5063.3311		11 mm (incl. 5 and 9 mm)**
		J5063.3313		13 mm (incl. 5, 9 and 11 mm)**
		J5064.3316*		16 mm
		J5063.4307	3.8 mm	7 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4309	3.8 mm	9 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4311	3.8 mm	11 mm (incl. 5 and 9 mm)**
			4.3 mm	
		J5063.4313	3.8 mm	13 mm (incl. 5, 9 and 11 mm)**
			4.3 mm	
		J5064.4316*	3.8 mm	16 mm
			4.3 mm	

* Necessary Guide System pilot drill for implant length 16 mm, following obligatory prior use of the pilot drill set length 13 mm.

** All Guide System pilot drill sets include a 5 mm long pilot drill, as well as all pilot drills necessary for the selected implant length.
 All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

	Article	Art. No.	Ø	L
	Guide System surgery set, SCREW-LINE internal irrigation, sterile Material Stainless steel	J5065.3309	3.3 mm	9 mm (incl. 5 mm)**
		J5065.3311		11 mm (incl. 5 and 9 mm)**
		J5065.3313		13 mm (incl. 5, 9 and 11 mm)**
		J5066.3316*		16 mm
		J5065.3807	3.8 mm	7 mm (incl. 5 mm)**
		J5065.3809		9 mm (incl. 5 mm)**
		J5065.3811		11 mm (incl. 5 and 9 mm)**
		J5065.3813		13 mm (incl. 5, 9 and 11 mm)**
		J5066.3816*		16 mm
		J5065.4307	4.3 mm	7 mm (incl. 5 mm)**
		J5065.4309		9 mm (incl. 5 mm)**
		J5065.4311		11 mm (incl. 5 and 9 mm)**
		J5065.4313		13 mm (incl. 5, 9 and 11 mm)**
		J5066.4316*		16 mm
	Guide System form drill, SCREW-LINE, cortical bone internal irrigation, sterile Material Stainless steel	J5068.3309	3.3 mm	9 mm
		J5068.3311		11 mm
		J5068.3313		13 mm
		J5068.3316		16 mm
		J5068.3807	3.8 mm	7 mm
		J5068.3809		9 mm
		J5068.3811		11 mm
		J5068.3813		13 mm
		J5068.3816		16 mm
		J5068.4307	4.3 mm	7 mm
		J5068.4309		9 mm
		J5068.4311		11 mm
		J5068.4313		13 mm
		J5068.4316		16 mm
	Guide System gingiva punch sterile Material Stainless steel	J5041.3303	3.3 mm	-
		J5041.3803	3.8 mm	
		J5041.4303	4.3 mm	

* Necessary Guide System form drill for implant length 16 mm, following obligatory prior use of the Guide System surgery set length 13 mm.

** All Guide System surgery sets include a 5 mm long pre-drill, as well as all form drills necessary for the selected implant length.

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

SCREW-LINE

Guide System

	Article	Art. No.	Ø	L
	Guide System guiding sleeve height 3.0 mm (2 units) Material Titanium alloy	J3734.3303*	3.3 mm	-
		J3734.3803*	3.8 mm	
		J3734.4303*	4.3 mm	
	Guide System CONELOG® Insertion post, screw-mounted for CONELOG® Lab implant/implant analog, incl. fixing screw (2 units) Material Titanium alloy	C2026.3303	3.3 mm	-
		C2026.3803	3.8 mm	
		C2026.4303	4.3 mm	
	Guide System template drill for Guide System guiding sleeve Material Stainless steel	J3733.3300	3.3 mm	-
		J3733.4300	3.8 mm	
			4.3 mm	
	Guide System seating tool for Guide System guiding sleeve Material Stainless steel	J3716.3300	3.3 mm	-
		J3716.4300	3.8 mm	
			4.3 mm	

* only for use with SCREW-LINE Implants with screw-mounted insertion post
All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

	Article	Art. No.	Ø	L
	Guide System check-up pin for Guide System guiding sleeve Material Stainless steel	J5301.3300	3.3 mm	-
		J5301.4300	3.8 mm	
			4.3 mm	
	Guide System driver* for Guide System implant Ø 3.3/3.8/4.3 mm, manual/wrench Material Stainless steel	J5303.4300	3.3 mm	-
			3.8 mm	
			4.3 mm	
	Guide System driver* for Guide System implant Ø 3.3/3.8/4.3 mm, with ISO shaft for angled hand piece Material Stainless steel	J5304.4300	3.3 mm	-
			3.8 mm	
			4.3 mm	
	Drill extension ISO shaft, for instruments with internal irrigation Material Stainless steel	J5002.0005	-	26.6 mm

* only for use with CONELOG® SCREW-LINE Implants with Art. No. C1063.xxxx.

General surgical instruments

	Article	Art. No.	Ø	L
	Round bur resterilizable Material Stainless steel	J5050.2300	2.3 mm	-
	Point drill resterilizable Material Stainless steel	B1012*	1.5 mm	30.0 mm
	Pilot drill without coil, resterilizable Material Stainless steel	J5051.2003	2.0 mm	-
	Pilot drill SCREW-LINE resterilizable Material Stainless steel	J5051.2000	2.0 mm	-
	Pre-drill SCREW-LINE resterilizable Material Stainless steel	J5051.2800	1.7 – 2.8 mm	-

* Manufacturer: AXIS biodental SA, Les Rosées 5, 2336 Les Bois, Switzerland

	Article	Art. No.	Ø	L
	Depth stop SCREW-LINE for pilot drill (J5051.2000) and pre-drill (J5051.2800), resterilizable Material Stainless steel	J5015.0007	-	7 mm
		J5015.0009		9 mm
		J5015.0011		11 mm
		J5015.0013		13 mm
	Bone profiler Material Stainless steel	Ø 5.0 mm J5003.3350	3.3 mm	-
		Ø 6.0 mm J5003.4360	3.8 mm 4.3 mm	
		Ø 7.0 mm J5003.5070	5.0 mm	
	CONELOG® Guiding pin for bone profiler Material Titanium alloy	C5002.3300	3.3 mm	-
		C5002.3800	3.8 mm	
		C5002.4300	4.3 mm	
		C5002.5000	5.0 mm	
	Countersink Material Stainless steel	Ø 4.6 mm J5006.3346	3.3 mm	-
		Ø 5.2 mm J5006.3852	3.8 mm	
		Ø 5.6 mm J5006.4356	4.3 mm	
		Ø 6.3 mm J5006.5063	5.0 mm	
	Baring drill for cover screw Material Stainless steel	J5004.3300	3.3 mm	-
		J5004.3800	3.8 mm	
		J5004.4300	4.3 mm	
		J5004.5000	5.0 mm	

General surgical instruments

	Article	Art. No.	Dimension
	Paralleling pin SCREW-LINE with depth marks Material Titanium alloy	J5300.2028	$\varnothing$ 1.7 – 2.8 mm/ 2.0 mm
	Drill extension ISO shaft (not for instruments with internal irrigation) Material Stainless steel	J5002.0006	26.5 mm
	Tap adapter, short for tap SCREW-LINE Material Stainless steel	J5322.0010	18.0 mm
	Tap adapter, long for tap SCREW-LINE Material Stainless steel	J5322.0011	23.0 mm

	Article	Art. No.	Dimension
	Driver, extra short for screw implants, manual/wrench Material Stainless steel	J5300.0031*	13.7 mm
	Driver, short for screw implants, manual/wrench Material Stainless steel	J5300.0032*	19.2 mm
	Driver, long for screw implants, manual/wrench Material Stainless steel	J5300.0033*	24.8 mm
	Driver, short for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft) Material Stainless steel	J5300.0036*	19.1 mm
	Driver, long for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft) Material Stainless steel	J5300.0037*	28.2 mm
	Driver, short for screw implants, with ISO-shaft for angled hand piece (with hexagon at the shaft) Material Stainless steel	J5300.0034*	19.1 mm
	Driver, long for screw implants, with ISO-shaft for angled hand piece (with hexagon at the shaft) Material Stainless steel	J5300.0035*	28.2 mm

* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1086.xxxx and CONELOG® SCREW-LINE Implants with Art. No. C1064.xxxx, C1065.xxxx and C1066.xxxx.

General surgical instruments

	Article	Art. No.	Dimension
	Cardanic driver (30°) for screw implants, adjustable length Material Stainless steel	J5300.0038*	-
	PickUp instrument holder for carrying implants Material Stainless steel	J5300.0030**	-
	Adapter ISO shaft for angled hand piece Material Stainless steel	J5002.0011	21.0 mm

* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1086.xxxx and CONELOG® SCREW-LINE Implants with Art. No. C1064.xxxx, C1065xxxx and C1066.xxxx.

** only for use with CONELOG® PROGRESSIVE-LINE Implants (with snap-in insertion post) with Art. No. C1086.xxxx and CONELOG® SCREW-LINE Implants with Art. No. C1062.xxxx and C1066.xxxx.

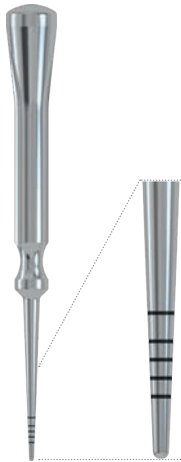
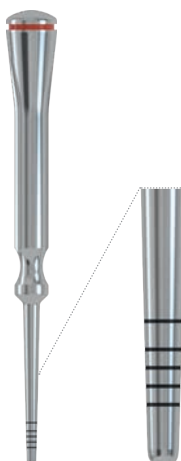
	Article	Art. No.	Ø	Dimension
	Holding key for insertion post Material Stainless steel	J5302.0010	-	-
	CONELOG® Adapter for screw implants, short for CONELOG® Implants Material Stainless steel	C5302.3311	3.3 mm	28.1 mm
		C5302.4311	3.8 mm	
			4.3 mm	
		C5302.5011	5.0 mm	
	CONELOG® Adapter for screw implants, long for CONELOG® Implants Material Stainless steel	C5302.3310	3.3 mm	33.1 mm
		C5302.4310	3.8 mm	
			4.3 mm	
	Holding sleeve for screw implants color-coded Material Titanium alloy	J5302.3300	3.3 mm	-
		J5302.3800	3.8 mm	
		J5302.4300	4.3 mm	
		J5302.5000	5.0 mm	
	Screwdriver hex, extra short, manual/wrench Material Stainless steel	J5317.0510	-	14.5 mm
	Screwdriver hex, short, manual/wrench Material Stainless steel	J5317.0501	-	22.5 mm
	Screwdriver hex, long, manual/wrench Material Stainless steel	J5317.0502	-	30.3 mm

General surgical instruments

	Article	Art. No.	Dimension
	Screwdriver hex, short, ISO shaft Material Stainless steel	J5317.0504	18.0 mm
	Screwdriver hex, long, ISO shaft Material Stainless steel	J5317.0503	26.0 mm
	Manual screwdriver, hex without wrench head connection Material Stainless steel	J5317.0511	23.0 mm
	Cleaning needle for instruments with internal irrigation Material Stainless steel	J5002.0012	-
	Cleaning cannula for drills with internal irrigation Material Stainless steel	J5002.0020	-

SCREW-LINE

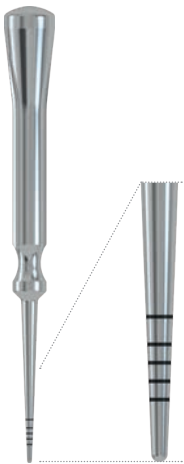
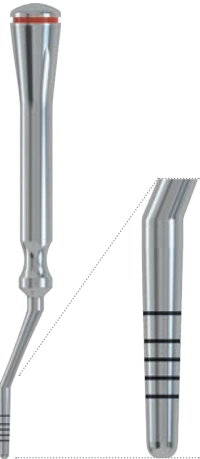
Osteotomy set

	Article	Art. No.	Ø
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight convex Material Stainless steel	J5418.0020	-
	Pre-Osteotome SCREW-LINE straight convex Material Stainless steel	J5417.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE straight convex Material Stainless steel	J5418.3300*	3.3 mm
		J5418.3800*	3.8 mm
		J5418.4300*	4.3 mm
		J5418.5000*	5.0 mm

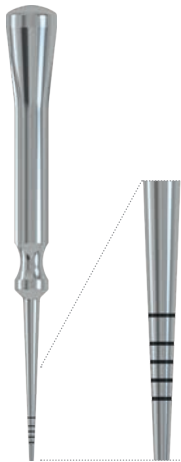
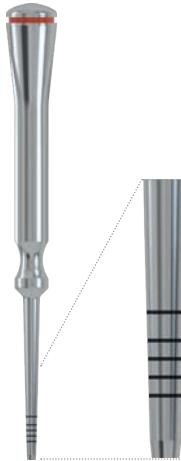
* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight convex.

SCREW-LINE

Osteotomy set

	Article	Art. No.	Ø
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex Material Stainless steel	J5418.0030	-
	Pre-Osteotome SCREW-LINE straight convex Material Stainless steel	J5417.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE angled convex Material Stainless steel	J5418.3310*	3.3 mm
		J5418.3810*	3.8 mm
		J5418.4310*	4.3 mm
		J5418.5010*	5.0 mm

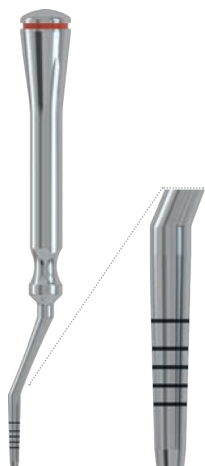
* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled convex.

	Article	Art. No.	Ø
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave Material Stainless steel	J5420.0020	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE straight concave Material Stainless steel	J5420.3300*	3.3 mm
		J5420.3800*	3.8 mm
		J5420.4300*	4.3 mm
		J5420.5000*	5.0 mm

* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE straight concave.

SCREW-LINE

Osteotomy set

	Article	Art. No.	Ø
	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave Material Stainless steel	J5420.0030	-
	Pre-Osteotome SCREW-LINE straight concave Material Stainless steel	J5419.2800*	1.7 – 2.8 mm
	Osteotome SCREW-LINE angled concave Material Stainless steel	J5420.3310*	3.3 mm
		J5420.3810*	3.8 mm
		J5420.4310*	4.3 mm
		J5420.5010*	5.0 mm

* These products are also included in the osteotomy set CAMLOG®/CONELOG® SCREW-LINE angled concave.

ALTApin set

	Article	Art. No.
	ALTApin set Membrane fixation system, resterilizable Material Plastic/Titanium alloy/Stainless steel	M5600.0110
	ALTApin tray (without content) Material Plastic	M5600.0210
	ALTApin applicator, straight inkl. aktivator Material Stainless steel	M5100.0010*
	ALTApin applicator, angled 90° inkl. aktivator Material Stainless steel	M5100.0030
	ALTApin applicator, straight, work element inkl. aktivator Material Stainless steel	M5200.0010

* These products are included in the ALTApin set.

ALTApin set

	Article	Art. No.
	ALTApin pricker Material Stainless steel	M5100.0050*
	ALTApin membrane fixator Material Stainless steel	M5100.0070*
	ALTApin surgery mallet Material Stainless steel/POM	M5100.0100
	ALTApin single patient drill, ISO shaft Material Stainless steel	M5500.0050
	ALTApin pricker, insert Material Stainless steel	M5200.0055*

* These products are included in the ALTApin set.

	Article	Art. No.
	ALTApin magazine 7 titanium pins, sterile, 1 unit	M1000.0050*
	Material Titanium alloy	
	ALTApin magazine 7 titanium pins, sterile, 3 units	M1000.0100
	Material Titanium alloy	

Cover screws

	Article	Art. No.	Ø
	CONELOG® Implant cover screw Material Titanium alloy	C2019.3300	3.3 mm
		C2019.3800	3.8 mm
		C2019.4300	4.3 mm
		C2019.5000	5.0 mm

Healing caps

	Article	Art. No.	Ø	GH	G Ø
	CONELOG® Healing cap, cylindrical sterile Material Titanium alloy	C2015.3320	3.3 mm	2.0 mm	3.0 mm
		C2015.3340		4.0 mm	3.0 mm
		C2015.3820	3.8 mm	2.0 mm	3.5 mm
		C2015.3840		4.0 mm	3.5 mm
		C2015.3860**	4.3 mm	6.0 mm	3.5 mm
		C2015.4320		2.0 mm	3.8 mm
		C2015.4340	5.0 mm	4.0 mm	3.8 mm
		C2015.4360**		6.0 mm	3.8 mm
		C2015.5020	5.0 mm	2.0 mm	4.5 mm
		C2015.5040		4.0 mm	4.5 mm
	CONELOG® Healing cap, wide body sterile Material Titanium alloy	C2014.3340	3.3 mm	4.0 mm	4.8 mm
		C2014.3840	3.8 mm	4.0 mm	5.3 mm
		C2014.3860		6.0 mm	5.3 mm
		C2014.4340	4.3 mm	4.0 mm	5.8 mm
		C2014.4360		6.0 mm	5.8 mm
		C2014.5040	5.0 mm	4.0 mm	6.5 mm
	CONELOG® Healing cap, bottleneck sterile Material Titanium alloy	C2014.5060		6.0 mm	6.5 mm
		C2011.3340	3.3 mm	4.0 mm	3.3 mm
		C2011.3840	3.8 mm	4.0 mm	3.8 mm
		C2011.3860		6.0 mm	3.8 mm
		C2011.4340	4.3 mm	4.0 mm	4.0 mm
		C2011.4360		6.0 mm	4.0 mm
		C2011.5040	5.0 mm	4.0 mm	4.7 mm
		C2011.5060		6.0 mm	4.7 mm

* These products are included in the ALTApin set.

** suitable for bite registration





Impression taking

	Article	Art. No.	Ø
 3 mm 10 mm	CONELOG® Impression posts, open tray incl. fixing screw (The fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex) Material Titanium alloy	C2121.3300	3.3 mm
		C2121.3800	3.8 mm
		C2121.4300	4.3 mm
		C2121.5000	5.0 mm
 10.7 mm	CONELOG® Impression posts, closed tray incl. impression cap, bite registration cap and fixing screw Material Titanium alloy/POM	C2110.3300	3.3 mm
		C2110.3800	3.8 mm
		C2110.4300	4.3 mm
		C2110.5000	5.0 mm
	Impression caps for impression post, closed tray (5 units) Material POM	J2111.3300	3.3 mm
		J2111.3800	3.8 mm
		J2111.4300	4.3 mm
		J2111.5000	5.0 mm

Bite registration

	Article	Art. No.	Ø
	CONELOG® Bite registration posts incl. fixing screw and bite registration cap Material Titanium alloy/POM	C2140.3300	3.3 mm
		C2140.3800	3.8 mm
		C2140.4300	4.3 mm
		C2140.5000	5.0 mm
	Bite registration caps (5 units) Material POM	J2112.3300	3.3 mm
		J2112.3800	3.8 mm
		J2112.4300	4.3 mm
		J2112.5000	5.0 mm

Fabrication of the plaster model

	Article	Art. No.	Ø
	CONELOG® Lab analog for cast models Material Titanium alloy	C3010.3300	3.3 mm
		C3010.3800	3.8 mm
		C3010.4300	4.3 mm
		C3010.5000	5.0 mm
	CONELOG® Implant analog for printed and cast models Material Titanium alloy	C3025.3300	3.3 mm
		C3025.3800	3.8 mm
		C3025.4300	4.3 mm
		C3025.5000	5.0 mm
	DIM Analog® for the CONELOG® Implant System for printed models, incl. thumbscrew Material Titanium alloy/Stainless steel	C3012.3300	3.3 mm
		C3012.4300	3.8 mm
			4.3 mm
		C3012.5000	5.0 mm

Manufacturer DIM Analog®: nt-trading GmbH & Co. KG, G.-Braun-Straße 18, 76187 Karlsruhe, Germany
 DIM Analog® is a registered trademark of nt-trading GmbH & Co. KG

Temporary restoration

	Article	Art. No.	Ø	GH
	CONELOG® Temporary abutment, crown, titanium alloy preparable, incl. abutment screw Material Titanium alloy	C2239.3300	3.3 mm*	-
		C2239.3800	3.8 mm	
		C2239.4300	4.3 mm	
		C2239.5000	5.0 mm	
	CONELOG® Temporary abutment, bridge, titanium alloy preparable, incl. abutment screw Material Titanium alloy	C2339.3300	3.3 mm	-
		C2339.3800	3.8 mm	
		C2339.4300	4.3 mm	
		C2339.5000	5.0 mm	

Esthomic® Abutments

Cemented crown and bridge restorations

	Article	Art. No.	Ø	GH
	CONELOG® Esthomic® Abutments, straight preparable, incl. abutment screw Material Titanium alloy	C2226.3815	3.8 mm	1.5 – 2.5 mm
		C2226.3830		3.0 – 4.5 mm
		C2226.4315	4.3 mm	1.5 – 2.5 mm
		C2226.4330		3.0 – 4.5 mm
		C2226.5015	5.0 mm	1.5 – 2.5 mm
		C2226.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, 15° angled, type A preparable, incl. abutment screw Material Titanium alloy	C2227.3815	3.8 mm	1.5 – 2.5 mm
		C2227.3830		3.0 – 4.5 mm
		C2227.4315	4.3 mm	1.5 – 2.5 mm
		C2227.4330		3.0 – 4.5 mm
		C2227.5015	5.0 mm	1.5 – 2.5 mm
		C2227.5030		3.0 – 4.5 mm

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

	Article	Art. No.	Ø	GH
	CONELOG® Esthomic® Abutments, 15° angled, type B preparable, incl. abutment screw Material Titanium alloy	C2228.3815	3.8 mm	1.5 – 2.5 mm
		C2228.3830		3.0 – 4.5 mm
		C2228.4315	4.3 mm	1.5 – 2.5 mm
		C2228.4330		3.0 – 4.5 mm
		C2228.5015	5.0 mm	1.5 – 2.5 mm
		C2228.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, 20° angled, type A preparable, incl. abutment screw Material Titanium alloy	C2231.3815	3.8 mm	1.5 – 2.5 mm
		C2231.3830		3.0 – 4.5 mm
		C2231.4315	4.3 mm	1.5 – 2.5 mm
		C2231.4330		3.0 – 4.5 mm
		C2231.5015	5.0 mm	1.5 – 2.5 mm
		C2231.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, 20° angled, type B preparable, incl. abutment screw Material Titanium alloy	C2232.3815	3.8 mm	1.5 – 2.5 mm
		C2232.3830		3.0 – 4.5 mm
		C2232.4315	4.3 mm	1.5 – 2.5 mm
		C2232.4330		3.0 – 4.5 mm
		C2232.5015	5.0 mm	1.5 – 2.5 mm
		C2232.5030		3.0 – 4.5 mm
	CONELOG® Esthomic® Abutments, Inset preparable, incl. abutment screw Material Titanium alloy	C2235.3320	3.3 mm*	2.0 – 3.3 mm
		C2235.3820	3.8 mm	
		C2235.4320	4.3 mm	
		C2235.5020	5.0 mm	

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

CAD/CAM prosthetics

Crown, bridge and hybrid restorations

	Article	Art. No.	Ø	GH
	CONELOG® Titanium bases CAD/CAM, crown bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2242.3308	3.3 mm*	0.8 mm
		C2242.3808	3.8 mm	
		C2242.4308	4.3 mm	
		C2242.5008	5.0 mm	
	CONELOG® Titanium bases CAD/CAM, crown bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2242.3320	3.3 mm*	2.0 mm
		C2242.3820	3.8 mm	
		C2242.4320	4.3 mm	
		C2242.5020	5.0 mm	
	CONELOG® Titanium bases CAD/CAM, bridge bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2342.3308	3.3 mm	0.8 mm
		C2342.3808	3.8 mm	
		C2342.4308	4.3 mm	
		C2342.5008	5.0 mm	
	CONELOG® Titanium bases CAD/CAM, bridge bonding base for individual CAD/CAM fabricated dental prosthesis, incl. dark purple anodized abutment screw and bonding aid (POM) Material Titanium alloy/POM	C2342.3320	3.3 mm	2.0 mm
		C2342.3820	3.8 mm	
		C2342.4320	4.3 mm	
		C2342.5020	5.0 mm	

The geometries of the CONELOG® Titanium bases CAD/CAM are available as a CAD library for leading dental CAD systems. The libraries are available for free download at: www.camlog.com/en/media-center/cad-libraries.

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

	Article	Art. No.	Ø	Thread
 11 mm	CONELOG® Modeling aids for CAMLOG® Titanium bases CAD/CAM burn-out, for fabricating mesostructures and crowns Material POM	C2242.3302	3.3 mm	-
		C2242.3802	3.8 mm	
		C2242.4302	4.3 mm	
		C2242.5002	5.0 mm	
	CONELOG® Abutment screw for CONELOG® Titanium bases CAD/CAM dark purple anodized Material Titanium alloy	C4015.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		C4015.2001	5.0 mm	M 2.0
	CONELOG® Lab screw for CONELOG® Titanium bases CAD/CAM brown partial anodized Material Titanium alloy	C4016.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		C4016.2001	5.0 mm	M 2.0
 10 mm	CONELOG® Scanbodies* for optical, 3-dimensional localization of CONELOG® Implants in the mouth or CONELOG® Lab analogs in the working model, incl. abutment screw, sterile Not compatible with the CEREC and inLab systems from Sirona® Material PEEK	C2600.3310	3.3 mm	-
		C2600.4310	3.8 mm	
			4.3 mm	
		C2600.5010	5.0 mm	
 10.2 mm	CONELOG® ScanPosts for Sirona® Scanbody for digital recording of the CONELOG® Implant or lab analog position and for further processing in the Sirona® CEREC and inLab systems, incl. abutment screw Material Titanium alloy	C2620.3306	3.3 mm	-
		C2620.3806	3.8 mm	
		C2620.4306	4.3 mm	
		C2620.5006	5.0 mm	

* Please check whether the CONELOG® Scanbody is available in the CAD software used. CAD libraries for selected CONELOG® Prosthetic components are available for free download at: www.camlog.com/en/media-center/cad-libraries

Matching Sirona® Scanbodies size S for CONELOG® ScanPosts and CONELOG® Titanium base CAD/CAM crown with Ø 3.3/3.8/4.3 mm:

For Omnicam®: Article number 6431311

For Bluecam®: Article number 6431295

Matching Sirona® Scanbodies size L for CONELOG® ScanPosts and CONELOG® Titanium base CAD/CAM crown with Ø 5.0 mm:

For Omnicam®: Article number 6431329

For Bluecam®: Article number 6431303

Sirona® Scanbodies are available from Dentsply Sirona®.

CAM titanium blanks

Milling production process of individualized one-piece abutments and healing caps by CAD/CAM technology

	Article	Art. No.	Ø
	CONELOG® CAM titanium blank, type IAC* Ø 12 mm, length 12.5 mm (2 units), sent with 2 separate packed abutment screws Material Titanium alloy	C2411.3313	3.3 mm
		C2411.4313	3.8 mm
			4.3 mm
		C2411.5013	5.0 mm
	CONELOG® CAM titanium blank, type ME** Ø 12 mm, length 20 mm (2 units), sent with 2 separate packed abutment screws Material Titanium alloy	C2421.3320	3.3 mm
		C2421.3820	3.8 mm
		C2421.4320	4.3 mm
		C2421.5020	5.0 mm

Accessories for CAM titanium blanks, type IAC

	Article	Art. No.	Ø
	CONELOG® Collet for CAM blank, type IAC* Ø 6 mm, length 17 mm, incl. 2 fixing screws for CAM blank, type IAC Material Stainless steel	C3720.3300	3.3 mm
		C3720.4300	3.8 mm
			4.3 mm
		C3720.5000	5.0 mm

Type IAC*

For the milling process, the CAM titanium blank type IAC is fixated to the implant-abutment connection via the CONELOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.

Type ME**

For the milling process, the CAM titanium blank type ME is fixated with the front-facing groove of its cylindrical section via a milling holder for PreFace® Abutments from Medentika®. These milling holders are available for selected machines from the particular machine manufacturer.

The CAM titanium blanks require product specific CAM libraries which are available on request for selected CAM softwares from the software provider.

The geometries of the CONELOG® CAM Titanium Blanks are available as a CAD library for leading dental CAD systems. The libraries are available for free download at:

www.camlog.com/en/media-center/cad-libraries.

Medentika® and Preface® are registered trademarks of Medentika GmbH, D-Hügelshheim.

Universal abutments

Cemented crown and bridge restorations

	Article	Art. No.	Ø	Dimension
	CONELOG® Universal abutments preparable, incl. abutment screw Material Titanium alloy	C2211.3300	3.3 mm*	-
		C2211.3800	3.8 mm	
		C2211.4300	4.3 mm	
		C2211.5000	5.0 mm	

Gold-plastic abutment

Cemented crown and bridge restorations

	Article	Art. No.	Ø	Noble metal weight
	CONELOG® Gold-plastic abutment cast-on, incl. abutment screw Material Cast-on gold alloy/POM	C2246.3300	3.3 mm*	ca. 0.31 g
		C2246.3800	3.8 mm	ca. 0.36 g
		C2246.4300	4.3 mm	ca. 0.36 g
		C2246.5000	5.0 mm	ca. 0.55 g

* only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)

Logfit® Prosthetic system

Cemented crown and bridge restorations


	Article	Art. No.	Ø	GH
	CONELOG® Logfit® Abutments incl. abutment screw Material Titanium alloy	C2550.3810	3.8 mm	1.0 mm
		C2550.3825		2.5 mm
		C2550.4310	4.3 mm	1.0 mm
		C2550.4325		2.5 mm
		C2550.5010	5.0 mm	1.0 mm
		C2550.5025		2.5 mm
	Logfit® Impression caps Material POM	J2551.4300	3.8 mm	-
			4.3 mm	
		J2551.6000	5.0 mm	
	Logfit® Analog Material Titanium alloy	J2552.4300	3.8 mm	-
			4.3 mm	
		J2552.6000	5.0 mm	
	Logfit® Plastic copings, for crowns (with rotation securing device) burn-out Material POM	J2553.4302	3.8 mm	-
			4.3 mm	
		J2553.6002	5.0 mm	
	Logfit® Plastic copings, for bridges (without rotation securing device) burn-out Material POM	J2553.4301	3.8 mm	-
			4.3 mm	
		J2553.6001	5.0 mm	

Occlusally screw-retained restorations

	Article	Art. No.	Typ	Ø	GH	PP Ø	
	CONELOG® Bar abutment, straight sterile Material Titanium alloy	C2254.3310	-	3.3 mm	1.0 mm	4.3 mm	
		C2254.3325			2.5 mm		
		C2254.3810		3.8 mm	1.0 mm	4.3 mm	
		C2254.3825			2.5 mm		
		C2254.3840			4.0 mm		
		C2254.4310		4.3 mm	1.0 mm	4.3 mm	
		C2254.4325			2.5 mm		
		C2254.4340			4.0 mm		
		C2254.5010		5.0 mm	1.0 mm	6.0 mm	
		C2254.5025			2.5 mm		
		C2254.5040			4.0 mm		
	CONELOG® Bar abutment, 17° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	C2256.3325	A	3.3 mm	2.5 mm	4.3 mm	
		C2256.3340			4.0 mm		
		C2257.3325	B		2.5 mm		4.0 mm
		C2257.3340			4.0 mm		
		C2256.3825	A	3.8 mm	2.5 mm	4.3 mm	
		C2256.3840			4.0 mm		
		C2257.3825	B		2.5 mm		4.0 mm
		C2257.3840			4.0 mm		
		C2256.4325	A	4.3 mm	2.5 mm	4.3 mm	
		C2256.4340			4.0 mm		
		C2257.4325	B		2.5 mm		4.0 mm
		C2257.4340			4.0 mm		
		C2256.5025	A	5.0 mm	2.5 mm	6.0 mm	
		C2256.5040			4.0 mm		
		C2257.5025	B		2.5 mm		4.0 mm
		C2257.5040			4.0 mm		
	CONELOG® Bar abutment, 30° angled incl. light blue anodized abutment screw with reduced head, sterile Material Titanium alloy	C2258.3325	A	3.3 mm	2.5 mm	4.3 mm	
		C2258.3340			4.0 mm		
		C2259.3325	B		2.5 mm		4.0 mm
		C2259.3340			4.0 mm		
		C2258.3825	A	3.8 mm	2.5 mm	4.3 mm	
		C2258.3840			4.0 mm		
		C2259.3825	B		2.5 mm		4.0 mm
		C2259.3840			4.0 mm		
		C2258.4325	A	4.3 mm	2.5 mm	4.3 mm	
		C2258.4340			4.0 mm		
		C2259.4325	B		2.5 mm		4.0 mm
		C2259.4340			4.0 mm		
		C2258.5035	A	5.0 mm	3.5 mm	6.0 mm	
		C2258.5050			5.0 mm		
		C2259.5035	B		3.5 mm		5.0 mm
		C2259.5050			5.0 mm		

Type A and B see on page 6

Occlusally screw-retained restorations




	Article	Art. No.	Ø	Dimension
	Orientation gauge for COMFOUR® for Ø 2.0 mm pilot drill hole Material Nitinol	J3551.0001	-	-
	Aligning tool for angled bar abutments, for insertion post	J2269.0003*	-	17°
		J2269.0004*	-	30°
	Material Stainless steel	J2269.0005**	-	17°
		J2269.0006**	-	30°
	Gingiva height indicator, straight Material Titanium alloy	J3550.3300	3.3 mm	-
		J3550.3800	3.8 mm	
		J3550.4300	4.3 mm	
		J3550.5000	5.0 mm	
	Driver for impression cap and healing cap for bar abutment Material Stainless steel	J5300.0027	3.3 mm 3.8 mm 4.3 mm	19.1 mm
		J5300.0028	5.0 mm	
	Healing cap for bar abutment partial light blue anodized, sterile Material Titanium alloy	J2029.4300	3.3 mm 3.8 mm 4.3 mm	-
		J2029.6000	5.0 mm	
	Impression cap, short, for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile Material Titanium alloy	J2129.4300	3.3 mm 3.8 mm 4.3 mm	6.5 mm
		J2129.6000	5.0 mm	7.0 mm
	Impression cap, long, for bar abutment, closed tray (bridge/bar) partial light blue anodized, sterile Material Titanium alloy	J2129.4310	3.3 mm 3.8 mm 4.3 mm	11.0 mm
		J2129.6010	5.0 mm	
	Bar lab analog for bar abutments Material Stainless steel	J3020.4300	3.3 mm 3.8 mm 4.3 mm	-
		J3020.6000	5.0 mm	
	Bar implant analog for bar abutments for printed and cast models Material Stainless steel	J3025.4300	3.3 mm 3.8 mm 4.3 mm	-
		J3025.6000	5.0 mm	
	Scanning cap for bar abutments incl. prosthetic screw, light blue anodized, sterile Material PEEK	J2610.4300	3.3 mm 3.8 mm 4.3 mm	-
		J2610.6000	5.0 mm	
	Titanium cap for bar abutment, for crown incl. prosthetic screw light blue anodized, sterile Material Titanium alloy	J2259.4301	3.3 mm 3.8 mm 4.3 mm	-
		J2259.6001	5.0 mm	

* only for use with CONELOG® Implants with Art. No. C1062.xxxx and C1063.xxxx.

** only for use with CONELOG® Implants with Art. No. C1064.xxxx and C1086.xxxx.

	Article	Art. No.	Ø			Dimension
	Titanium cap for bar abutment, for bridge incl. prosthetic screw light blue anodized, sterile	J2259.4302	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6002	5.0 mm			
	Titanium cap without retention for bar abutment, for bridge incl. prosthetic screw light blue anodized	J2259.4322	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2259.6022	5.0 mm			
	Crown base for bar abutment burn-out	J2256.4306	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2256.6006	5.0 mm			
	Base for bar abutment burn-out	J2257.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2257.6001	5.0 mm			
	Base for bar abutment cast-on	J2263.4300	3.3 mm	3.8 mm	4.3 mm	ca. 0.48 g
	Material Cast-on gold alloy/POM	J2263.6000	5.0 mm			ca. 0.70 g
	Base for bar abutment solderable	J2258.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Solderable gold alloy	J2258.6000	5.0 mm			
	Base for bar abutment, titanium laser-weldable	J2262.4300	3.3 mm	3.8 mm	4.3 mm	-
	Material Titan Grade 4	J2262.6000	5.0 mm			
	Titanium bonding base for bar abutment Passive-Fit	J2260.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy	J2260.6001	5.0 mm			
	Bar sleeve for titanium bonding base burn-out, Passive-Fit, incl. prosthetic screw for bar abutments, hex (only for fabrication of the cast framework in conjunction with bar sleeves for titanium bonding base Passive-Fit)	J2261.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material POM	J2261.6001	5.0 mm			
	Polishing protection for caps and bases for bar abutment	J3021.4300	3.3 mm	3.8 mm	4.3 mm	Thread M 1.6
	Material Titanium alloy	J3021.6000	5.0 mm			Thread M 2.0

Occlusally screw-retained restorations

	Article	Art. No.	Ø			Thread
	Locator® Fixture for bar abutment	J2253.4301	3.3 mm	3.8 mm	4.3 mm	-
	Material Titanium alloy/TiN	J2253.6001	5.0 mm			
	CONELOG® Abutment screw with reduced head, hex, light blue anodized	C4004.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	C4004.2001	5.0 mm			M 2.0
	CONELOG® Lab screw reduced head, hex, partial light blue anodized	C4004.1600	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	C4004.2000	5.0 mm			M 2.0
	Prosthetic screw for bar abutments hex, light blue anodized (for final fixation of the restoration)	J4012.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4012.2001	5.0 mm			M 2.0
	Lab prosthetic screw for bar abutment hex, brown anodized	J4013.1601	3.3 mm	3.8 mm	4.3 mm	M 1.6
	Material Titanium alloy	J4013.2001	5.0 mm			M 2.0
	Screw, hex, length 10 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1610	-			M 1.6
	Material Titanium alloy	J4012.2010				M 2.0
	Screw, hex, length 15 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1615	-			M 1.6
	Material Titanium alloy	J4012.2015				M 2.0
	Screw, hex, length 20 mm can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1620	-			M 1.6
	Material Titanium alloy	J4012.2020				M 2.0

Lab screws may not be used on patients.

	Article	Art. No.	Ø	Thread
	Plastic screw for bar abutment hex, length 27 mm, sterile Material PEEK	J4009.1627	-	M 1.6
		J4009.2027		M 2.0

Ball abutment anchoring system

	Article	Art. No.	Ø	GH
	CONELOG® Ball abutment male part incl. stabilizing ring Material Titanium alloy/Plastic	C2249.3315	3.3 mm	1.5 mm
		C2249.3330		3.0 mm
		C2249.3815	3.8 mm	1.5 mm
		C2249.3830		3.0 mm
		C2249.3845	4.3 mm	4.5 mm
		C2249.4315		1.5 mm
		C2249.4330	5.0 mm	3.0 mm
		C2249.4345		4.5 mm
		C2249.5015	5.0 mm	1.5 mm
		C2249.5030		3.0 mm
		C2249.5045		4.5 mm
	Matrix CM Dalbo®-Plus for ball abutment, incl. lamella retention insert Material Titanium Grade 4/Gold alloy	05003503	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Lamella retention insert for matrix CM Dalbo®-Plus Material Gold alloy	05003504	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Biel, Switzerland.

Ball abutment anchoring system

	Article	Art. No.	Ø	GH
	Ball abutment analogs incl. stabilizing ring Material Brass/Plastic	C3015.3300	3.3 mm	-
			3.8 mm	
			4.3 mm	
		C3015.5000	5.0 mm	

Locator® Anchoring system

CONELOG® Locator R-Tx®

	Article	Art. No.	Ø	GH
	CONELOG® Locator R-Tx® Abutment incl. titanium housing with processing replacement male black, block-out spacer white and four different retention inserts Material Titanium alloy/Nylon	30805-01	3.3 mm	1.0 mm
		30805-02		2.0 mm
		30805-03		3.0 mm
		30805-04		4.0 mm
		30806-01	3.8 mm	1.0 mm
		30806-02		2.0 mm
		30806-03		3.0 mm
		30806-04		4.0 mm
		30806-05		5.0 mm
		30807-01	4.3 mm	1.0 mm
		30807-02		2.0 mm
		30807-03		3.0 mm
		30807-04		4.0 mm
		30807-05		5.0 mm
		30808-01	5.0 mm	1.0 mm
		30808-02		2.0 mm
		30808-03		3.0 mm
		30808-04		4.0 mm
		30808-05		5.0 mm
	Locator R-Tx® Impression coping (4 units) Material Polyethylene	30017-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator R-Tx® Analog Ø 3.35 mm (4 units) Material Aluminum	30014-01	3.3 mm	-
			3.8 mm	
			4.3 mm	

	Article	Art. No.	Ø	GH
	Locator R-Tx® Analog Ø 5.0 mm (4 units) Material Aluminum	30016-01	5.0 mm	-
	Locator R-Tx® Titanium housing with processing insert black (4 units) Material Titanium alloy/Polyethylene	30013-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Processing insert black (4 units) Material Polyethylene	30012-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Processing spacer (4 units) Material Polyethylene	30018-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Retention insert gray, ZERO RETENTION (4 units) Material Nylon	30001-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Retention insert blue, LIGHT (4 units) Material Nylon	30002-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-
	Locator R-Tx® Retention insert pink, MEDIUM (4 units) Material Nylon	30003-01	3.3 mm 3.8 mm 4.3 mm 5.0 mm	-

Locator® Anchoring system

CONELOG® Locator R-Tx®

	Article	Art. No.	Ø	GH
	Locator R-Tx® Retention insert white, STRONG (4 units) Material Nylon	30004-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

Locator® Anchoring system

CONELOG® Locator®

	Article	Art. No.	Ø	GH
	CONELOG® Locator® Abutment Material Titanium alloy/TiN	C2253.3310	3.3 mm	1.0 mm
		C2253.3320		2.0 mm
		C2253.3330		3.0 mm
		C2253.3340		4.0 mm
		C2253.3810	3.8 mm	1.0 mm
		C2253.3820		2.0 mm
		C2253.3830		3.0 mm
		C2253.3840		4.0 mm
		C2253.3850		5.0 mm
		C2253.4310	4.3 mm	1.0 mm
		C2253.4320		2.0 mm
		C2253.4330		3.0 mm
		C2253.4340		4.0 mm
		C2253.4350		5.0 mm
		C2253.5010	5.0 mm	1.0 mm
		C2253.5020		2.0 mm
		C2253.5030		3.0 mm
		C2253.5040		4.0 mm
		C2253.5050		5.0 mm
	Locator® Impression cap (4 units) Material Aluminum/Polyethylene	J2253.0200	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	Locator® Analog (4 units) Material Aluminum	J2253.0340	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

	Article	Art. No.	Ø
	Locator® Male processing package (2 units) Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male clear 1 Replacement male pink 1 Replacement male blue Material Titanium alloy/Polyethylene/Teflon/Nylon	J2253.0102	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Male processing package for extended range (2 units) Content per package: 1 Titanium housing with processing replacement male 1 Block out spacer white 1 Replacement male green, 1 Replacement male orange, 1 Replacement male red Material Titanium alloy/Polyethylen/Teflon/Nylon	J2253.0112	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Block out spacer (20 units) Material Teflon	J2253.0401	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Processing replacement male (4 units) Material Polyethylen	J2253.0402	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male clear, STRONG, Div.: 0°-10° (4 units) Material Nylon	J2253.1005	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

Locator® Anchoring system

CONELOG® Locator®

	Article	Art. No.	Ø
	Locator® Replacement male pink, MEDIUM, Div.: 0° – 10° (4 units) Material Nylon	J2253.1003	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male blue, LIGHT, Div.: 0° – 10° (4 units) Material Nylon	J2253.1002	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* green, STRONG, Div.: 10° – 20° (4 units) Material Nylon	J2253.2004	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* orange, MEDIUM, Div.: 10° – 20° (4 units) Material Nylon	J2253.2003	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* red, LIGHT, Div.: 10° – 20° (4 units) Material Nylon	J2253.2002	3.8 mm
			4.3 mm
			5.0 mm
	Locator® Replacement male for extended range* gray, NO RETENTION, Div.: 0° – 20° (4 units) Material Nylon	J2253.2000	3.8 mm
			4.3 mm
			5.0 mm

* not permitted for implant Ø 3.3 mm

Manufacturer Locator®: Zest Anchors, 2875 Loker Avenue East, Carlsbad, California 92010, USA

Locator® and Locator R-Tx® are registered trademarks of Zest Anchors

Double crown restoration

	Article	Art. No.	Ø
 11 mm	CONELOG® Universal abutments for double crown restorations preparable, incl. abutment screw Material Titanium alloy	C2211.3800	3.8 mm
		C2211.4300	4.3 mm
		C2211.5000	5.0 mm
 12 mm	CONELOG® Telescope abutments for double crown restorations preparable, incl. abutment screw Material Titanium alloy	C2212.3800	3.8 mm
		C2212.4300	4.3 mm
		C2212.5000	5.0 mm

Accessories for abutments

	Article	Art. No.	Ø	Thread
	CONELOG® Abutment screw, hex for definitive screw retention of abutments into the implant Material Titanium alloy	C4005.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		C4005.2001	5.0 mm	M 2.0
	CONELOG® Lab screw, hex for the fixation of abutments on the working model, brown anodized Material Titanium alloy	C4006.1601	3.3 mm	M 1.6
			3.8 mm	
			4.3 mm	
		C4006.2001	5.0 mm	M 2.0

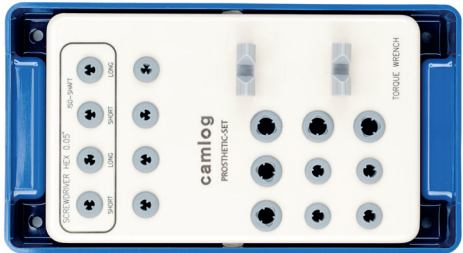
Lab screws may not be used on patients.

Prosthetic instruments

	Article	Art. No.	L
	Torque wrench with continuous torque adjustment until maximal 30 Ncm Material Stainless steel	J5320.1030	-
	Driver for ball abutment, manual/wrench Material Stainless steel	J5300.0011	18.3 mm
	Screwdriver Activator for ball abutment matrix CM Dalbo®-Plus Material Stainless steel	07000389	-
	Driver for straight bar abutment, short Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0020	18.6 mm
	Driver for straight bar abutment, short Ø 5.0 mm Material Stainless steel	J5300.0025	18.6 mm

	Article	Art. No.	L
	Driver for straight bar abutment, long Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0021	28.0 mm
	Driver for impression cap and healing cap for bar abutment Ø 3.3/3.8/4.3 mm Material Stainless steel	J5300.0027	19.1 mm
	Driver for impression cap and healing cap for bar abutment Ø 5.0 mm Material Stainless steel	J5300.0028	19.1 mm
	Driver for Locator®, manual/wrench Material Stainless steel	J2253.0001	24.3 mm
	Locator® Instrument threepart Material Stainless steel	J2253.0002	83.0 mm
	Locator® Abutment holder sleeve for golden component of the Locator® Instrument (4 units) Material Polysulfone	08394	-
	Locator® Angle measurement guide Material Stainless steel	J2253.0003	-
	Locator® Parallel post (4 units) Material Polyethylene	J2253.0004	-

Prosthetic instruments

	Article	Art. No.	L
	Locator R-Tx® Retention insert tool with plastic grip Material Stainless steel	30021-01	
	Prosthetic set Content: - J5320.1030 Torque wrench - J5317.0501 Screwdriver, hex, short, manual/wrench - J5317.0502 Screwdriver, hex, long, manual/wrench - J5317.0504 Screwdriver, hex, short, ISO shaft - J5317.0503 Screwdriver, hex, long, ISO shaft	J5330.8600	197 x 108 x 54 mm
	Prosthetic tray (without content) Material Plastic	J5330.8500	197 x 108 x 54 mm
	Prosthetic tray universal (without content) resterilizable Material Radel®/Silicone	J5330.8700	162 x 73 x 29 mm
	Screwdriver Hex, extra short, manual/wrench Material Stainless steel	J5317.0510	14.5 mm
	Screwdriver Hex, short, manual/wrench Material Stainless steel	J5317.0501	22.5 mm

	Article	Art. No.	Ø	Dimension
	Screwdriver Hex, long, manual/wrench Material Stainless steel	J5317.0502	-	30.3 mm
	Screwdriver Hex, short, ISO shaft Material Stainless steel	J5317.0504	-	18.0 mm
	Screwdriver Hex, long, ISO shaft Material Stainless steel	J5317.0503	-	26.0 mm
	Manual screwdriver Hex, without wrench head connection Material Stainless steel	J5317.0511	-	23.0 mm
	Handle for CAMLOG®/CONELOG® Implant analog Material Stainless steel	J3025.0010	3.3 mm	-
		J3025.0015	5.0 mm	
	CONELOG® Disconnecter for CONELOG® Abutments, short Material Stainless steel	C5300.1601	3.3 mm	Thread M 1.6
			4.3 mm	
		C5300.2001	5.0 mm	Thread M 2.0
	CONELOG® Disconnecter for CONELOG® Abutments, long Material Stainless steel	C5300.1603	3.3 mm	Thread M 1.6
			4.3 mm	
		C5300.2003	5.0 mm	Thread M 2.0

Instruments for dental technicians

	Article	Art. No.	Ø
	Universal holder incl. 2 CONELOG® Lab screws, hex, and 1 CONELOG® Abutment collet each for Ø 3.3/3.8/4.3/5.0 mm Material Stainless steel/Titanium alloy	C3709.0010	-
	Universal holder Material Stainless steel	J3709.0015	-
	CONELOG® Abutment collets for universal holder, for grinding CAMLOG® Abutments Material Titanium alloy	C3709.3300	3.3 mm
		C3709.3800	3.8 mm
		C3709.4300	4.3 mm
		C3709.5000	5.0 mm
	Reworking reamer, for base for bar abutment plane surface, burn-out Material Stainless steel/Brass	J3711.0010	3.3 mm 3.8 mm 4.3 mm
		J3711.0015	5.0 mm
	Reworking reamer, for base for bar abutment screw seat, burn-out Material Stainless steel/Brass	J3711.0020	3.3 mm 3.8 mm 4.3 mm
		J3711.0025	5.0 mm

Selection abutments

	Article	Art. No.
 The image shows a grey plastic case for the CONELOG Selection abutment kit. The lid is open, revealing a grid of compartments containing various colored abutments (yellow, red, blue, and white). The lid has the CONELOG logo and a caution note in German and English: 'Caution: Do not use chairside! Achtung: Nicht zur Verwendung im Patientenzimmer bestimmt!'.	CONELOG® Selection abutment kit (Content: 2 units each, according table below)	C8011.1000

Content: CONELOG® Selection abutment kit					
Article	Material	Ø			GH
CONELOG® Esthomic® Selection abutment, straight*	POM	3.8 mm	4.3 mm	5.0 mm	1.5 – 2.5 mm
CONELOG® Esthomic® Selection abutment, 15° angled, type A*					3.0 – 4.5 mm
CONELOG® Esthomic® Selection abutment, 15° angled, type B*					1.5 – 2.5 mm
CONELOG® Esthomic® Selection abutment, 20° angled, type A*					
CONELOG® Esthomic® Selection abutment, 20° angled, type B*					

Attention, do not use selection abutments on patients!

* These products are not available singly.





Implants for practice

	Article	Art. No.	Ø	L
	CONELOG® PROGRESSIVE-LINE Implant for practice incl. snap-in insertion post and cover screw, yellow anodized Material Titanium alloy	C1901.3813	3.8 mm	13 mm
	CONELOG® PROGRESSIVE-LINE Implant for practice incl. snap-in insertion post and cover screw, red anodized Material Titanium alloy	C1901.4313	4.3 mm	
	CONELOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, yellow anodized Material Titanium alloy	C1069.3813	3.8 mm	13 mm
	CONELOG® SCREW-LINE Implant for practice incl. insertion post and cover screw, red anodized Material Titanium alloy	C1069.4313	4.3 mm	

Attention, do not use implants for practice on patients!

Demonstration models

	Article	Art. No.
	CONELOG® Demonstration model, acrylic glass upper jaw, 4 CONELOG® SCREW-LINE Implants, 4 x Ø 4.3 mm Material Acrylic glass/Titanium	C8070.1020
	CONELOG® Demonstration model, acrylic glass lower jaw, 4 CONELOG® SCREW-LINE Implants, 4 x Ø 4.3 mm Material Acrylic glass/Titanium	C8050.1040
	Edentulous mandible incl. mounting plate Material Plastic	J8070.2050

Macro models

	Article	Art. No.
	CONELOG® PROGRESSIVE-LINE Macro model Scale 3:1 Content: 1 CONELOG® PROGRESSIVE-LINE Implant 1 CONELOG® Esthomic® Abutment, straight 1 CONELOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic socket Material Plastic/Stainless steel	C8010.1400
	CONELOG® SCREW-LINE Macro model Scale 3:1 Content: 1 CONELOG® SCREW-LINE Implant 1 CONELOG® Esthomic® Abutment, straight 1 CONELOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic socket Material Plastic/Stainless steel	C8010.1010

Literature

	Article	Art. No.
	Patient brochure Questions and answers to dental implants	-
	COMFOUR® Patient brochure Bridge instead of dentures – dental prosthesis with feel-good factor	-
	Implant pass Patient-specific documentation of implant restoration Packaging units: 10 units	-
	Patient advice sheets Set á 5 sheets, A4	-
	Presentation folder A4, laminated	-

	Article	Art. No.
	Poster Format: 50 x 70 cm	-
	Appointment pad 50 sheets/pad, A7 Packaging units: 5 units	-

Indication overview

Single tooth restoration		Bridge restoration
Cemented	Screwed	Cemented
	 Temporary abutment, crown, titanium alloy	
 Esthomic® Abutments		 Esthomic® Abutments
	 Bar abutments	
 Titanium bases CAD/CAM, crown	 Titanium bases CAD/CAM, crown	 Titanium bases CAD/CAM, bridge
 Logfit® Abutment		 Logfit® Abutment
  Universal abutment CAM titanium blank		  Universal abutment CAM titanium blank
 Gold-plastic abutment	 Gold-plastic abutment	 Gold-plastic abutment

Bridge restoration	Hybrid restoration
Screwed	Removable (full denture)
 Temporary abutment, bridge, titanium alloy	
 Bar abutments	 Bar abutments
 Titanium bases CAD/CAM, bridge	
	 Locator® Anchoring system
	 Ball abutment
Double crown restoration	  Universal abutment CAM titanium blank
	 Telescope abutment
	 Gold-plastic abutment
	 Titanium bases CAD/CAM, crown



Implant overview

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No. A Ø				L
 CONELOG® PROGRESSIVE-LINE Implant, Promote® plus with screw-mounted insertion post	-		C1085.3807 A Ø 3.0 mm	C1085.4307 A Ø 3.0 mm	C1085.5007 A Ø 3.5 mm	7 mm
	C1085.3309 A Ø 2.2 mm		C1085.3809 A Ø 3.0 mm	C1085.4309 A Ø 3.0 mm	C1085.5009 A Ø 3.5 mm	9 mm
	C1085.3311 A Ø 2.2 mm		C1085.3811 A Ø 2.7 mm	C1085.4311 A Ø 2.7 mm	C1085.5011 A Ø 3.2 mm	11 mm
	C1085.3313 A Ø 2.2 mm		C1085.3813 A Ø 2.7 mm	C1085.4313 A Ø 2.7 mm	C1085.5013 A Ø 3.2 mm	13 mm
	C1085.3316 A Ø 2.2 mm		C1085.3816 A Ø 2.7 mm	C1085.4316 A Ø 2.7 mm	C1085.5016 A Ø 3.2 mm	16 mm
 CONELOG® PROGRESSIVE-LINE Implant, Promote® plus with snap-in insertion post	-		C1086.3807 A Ø 3.0 mm	C1086.4307 A Ø 3.0 mm	C1086.5007 A Ø 3.5 mm	7 mm
	C1086.3309 A Ø 2.2 mm		C1086.3809 A Ø 3.0 mm	C1086.4309 A Ø 3.0 mm	C1086.5009 A Ø 3.5 mm	9 mm
	C1086.3311 A Ø 2.2 mm		C1086.3811 A Ø 2.7 mm	C1086.4311 A Ø 2.7 mm	C1086.5011 A Ø 3.2 mm	11 mm
	C1086.3313 A Ø 2.2 mm		C1086.3813 A Ø 2.7 mm	C1086.4313 A Ø 2.7 mm	C1086.5013 A Ø 3.2 mm	13 mm
	C1086.3316 A Ø 2.2 mm		C1086.3816 A Ø 2.7 mm	C1086.4316 A Ø 2.7 mm	C1086.5016 A Ø 3.2 mm	16 mm

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		A Ø 2.7 mm	A Ø 3.5 mm	A Ø 3.9 mm	A Ø 4.6 mm	
Article		Art. No.				L
 CONELOG® SCREW-LINE Implant, Promote® plus with snap-in insertion post	-		C1066.3807	C1066.4307	C1066.5007	7 mm
	C1066.3309		C1066.3809	C1066.4309	C1066.5009	9 mm
	C1066.3311		C1066.3811	C1066.4311	C1066.5011	11 mm
	C1066.3313		C1066.3813	C1066.4313	C1066.5013	13 mm
	C1066.3316		C1066.3816	C1066.4316	C1066.5016	16 mm
 CONELOG® SCREW-LINE Implant, Promote® plus with screw-mounted insertion post	-		C1065.3807	C1065.4307	C1065.5007	7 mm
	C1065.3309		C1065.3809	C1065.4309	C1065.5009	9 mm
	C1065.3311		C1065.3811	C1065.4311	C1065.5011	11 mm
	C1065.3313		C1065.3813	C1065.4313	C1065.5013	13 mm
	C1065.3316		C1065.3816	C1065.4316	C1065.5016	16 mm

Prosthetics overview

Impression taking

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Impression posts, open tray	C2121.3300	C2121.3800	C2121.4300	C2121.5000	-
	CONELOG® Impression posts, closed tray	C2110.3300	C2110.3800	C2110.4300	C2110.5000	-
	Impression caps for impression post, closed tray	J2111.3300	J2111.3800	J2111.4300	J2111.5000	-

Bite registration

	CONELOG® Bite registration posts incl. fixing screw and bite registration cap	C2140.3300	C2140.3800	C2140.4300	C2140.5000	-
---	--	------------	------------	------------	------------	---

Fabrication of the plaster model

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Lab analogs, for cast models	C3010.3300	C3010.3800	C3010.4300	C3010.5000	-
	CONELOG® Implant analog, for printed and cast models	C3025.3300	C3025.3800	C3025.4300	C3025.5000	-
	DIM Analog® for printed models, for the CONELOG® Implant System	C3012.3300	C3012.4300	C3012.4300	C3012.5000	-

Abutments for crown and bridge restoration

	CONELOG® Temporary abutments, crown, titanium alloy	C2239.3300	C2239.3800	C2239.4300	C2239.5000	-
	CONELOG® Temporary abutments, bridge, titanium alloy	C2339.3300	C2339.3800	C2339.4300	C2339.5000	-
	CONELOG® Esthomic® Abutments, straight	-	C2226.3815	C2226.4315	C2226.5015	1.5 – 2.5
			C2226.3830	C2226.4330	C2226.5030	3.0 – 4.5
	CONELOG® Esthomic® Abutments, 15° angled, type A	-	C2227.3815	C2227.4315	C2227.5015	1.5 – 2.5
			C2227.3830	C2227.4330	C2227.5030	3.0 – 4.5
	CONELOG® Esthomic® Abutments, 15° angled, type B	-	C2228.3815	C2228.4315	C2228.5015	1.5 – 2.5
			C2228.3830	C2228.4330	C2228.5030	3.0 – 4.5
	CONELOG® Esthomic® Abutments, 20° angled, type A	-	C2231.3815	C2231.4315	C2231.5015	1.5 – 2.5
			C2231.3830	C2231.4330	C2231.5030	3.0 – 4.5
	CONELOG® Esthomic® Abutments, 20° angled, type B	-	C2232.3815	C2232.4315	C2232.5015	1.5 – 2.5
			C2232.3830	C2232.4330	C2232.5030	3.0 – 4.5

Prosthetics overview

Abutments for crown and bridge restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Esthomic® Abutments Inset	C2235.3320	C2235.3820	C2235.4320	C2235.5020	2.0 – 3.3 mm
	CONELOG® Universal abutments	C2211.3300	C2211.3800	C2211.4300	C2211.5000	-
	CONELOG® Gold-plastic abutments	C2246.3300	C2246.3800	C2246.4300	C2246.5000	-
	CONELOG® Titanium bases CAD/CAM, crown	C2242.3308	C2242.3808	C2242.4308	C2242.5008	0.8 mm
		C2242.3320	C2242.3820	C2242.4320	C2242.5020	2.0 mm
	CONELOG® Titanium bases CAD/CAM, bridge	C2342.3308	C2342.3808	C2342.4308	C2342.5008	0.8 mm
		C2342.3320	C2342.3820	C2342.4320	C2342.5020	2.0 mm
	CONELOG® Logfit® Abutments	-	C2550.3810	C2550.4310	C2550.5010	1.0 mm
			C2550.3825	C2550.4325	C2550.5025	2.5 mm
	Logfit® Impression caps	-	J2551.4300	J2551.4300	J2551.6000	-
	Logfit® Analog	-	J2552.4300	J2552.4300	J2552.6000	-
	Logfit® Plastic copings, for crowns	-	J2553.4302	J2553.4302	J2553.6002	-
	Logfit® Plastic copings, for bridges	-	J2553.4301	J2553.4301	J2553.6001	-

COMFOUR® Abutments for crown, bridge and hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Bar abutment, straight	C2254.3310	C2254.3810	C2254.4310	C2254.5010	1.0 mm
		C2254.3325	C2254.3825	C2254.4325	C2254.5025	2.5 mm
		-	C2254.3840	C2254.4340	C2254.5040	4.0 mm
	CONELOG® Bar abutment, 17° angled, type A	C2256.3325	C2256.3825	C2256.4325	C2256.5025	2.5 mm
		C2256.3340	C2256.3840	C2256.4340	C2256.5040	4.0 mm
	CONELOG® Bar abutment, 17° angled, type B	C2257.3325	C2257.3825	C2257.4325	C2257.5025	2.5 mm
		C2257.3340	C2257.3840	C2257.4340	C2257.5040	4.0 mm
	CONELOG® Bar abutment, 30° angled, Type A	C2258.3325	C2258.3825	C2258.4325	C2258.5035*	2.5 mm/ 3.5 mm*
		C2258.3340	C2258.3840	C2258.4340	C2258.5050*	4.0 mm/ 5.0 mm*
	CONELOG® Bar abutment, 30° angled, Type B	C2259.3325	C2259.3825	C2259.4325	C2259.5035*	2.5 mm/ 3.5 mm*
		C2259.3340	C2259.3840	C2259.4340	C2259.5050*	4.0 mm/ 5.0 mm*
	Healing cap for bar abutment	J2029.4300	J2029.4300	J2029.4300	J2029.6000	-
	Impression cap, short, for bar abutment, closed tray	J2129.4300	J2129.4300	J2129.4300	J2129.6000	-
	Impression cap, long, for bar abutment, closed tray (bridge/bar)	J2129.4310	J2129.4310	J2129.4310	J2129.6010	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-
	Titanium cap for bar abutment, for crown	J2259.4301	J2259.4301	J2259.4301	J2259.6001	-
	Titanium cap for bar abutment, for bridge	J2259.4302	J2259.4302	J2259.4302	J2259.6002	-
	Titanium cap without retention for bar abutment, for bridge	J2259.4322	J2259.4322	J2259.4322	J2259.6022	-
	Crown base for bar abutment, burn-out	J2256.4306	J2256.4306	J2256.4306	J2256.6006	-
	Base for bar abutment, burn-out	J2257.4301	J2257.4301	J2257.4301	J2257.6001	-
	Base for bar abutment, cast-on	J2263.4300	J2263.4300	J2263.4300	J2263.6000	-


Prosthetics overview

COMFOUR® Abutments for crown, bridge and hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	Base for bar abutment, solderable	J2258.4300	J2258.4300	J2258.4300	J2258.6000	-
	Base for bar abutment, titanium, laser-weldable	J2262.4300	J2262.4300	J2262.4300	J2262.6000	-
	Titanium bonding base for bar abutment, Passive-Fit	J2260.4301	J2260.4301	J2260.4301	J2260.6001	-
	Sleeve for titanium bonding base, burn-out, Passive-Fit	J2261.4301	J2261.4301	J2261.4301	J2261.6001	-
	Locator® Fixture for bar abutment	J2253.4301	J2253.4301	J2253.4301	J2253.6001	-

Hybrid restoration

	CONELOG® Ball abutment, male part	C2249.3315	C2249.3815	C2249.4315	C2249.5015	1.5 mm
		C2249.3330	C2249.3830	C2249.4330	C2249.5030	3.0 mm
		-	C2249.3845	C2249.4345	C2249.5045	4.5 mm
	Matrix CM Dalbo®-Plus	05003503	05003503	05003503	05003503	-
	Ball abutment analog	C3015.3300	C3015.3300	C3015.3300	C3015.5000	-
	CONELOG® Locator R-Tx® Abutment	30805-01	30806-01	30807-01	30808-01	1.0 mm
		30805-02	30806-02	30807-02	30808-02	2.0 mm
		30805-03	30806-03	30807-03	30808-03	3.0 mm
		30805-04	30806-04	30807-04	30808-04	4.0 mm
		-	30806-05	30807-05	30808-05	5.0 mm
	Locator R-Tx® Impression coping	30017-01	30017-01	30017-01	30017-01	-
	Locator R-Tx® Analog	30014-01	30014-01	30014-01	30016-01	-
	Locator R-Tx® Titanium housing	30013-01	30013-01	30013-01	30013-01	-
	Locator R-Tx® Processing insert	30012-01	30012-01	30012-01	30012-01	-
	Locator R-Tx® Processing spacer	30018-01	30018-01	30018-01	30018-01	-
	Locator R-Tx® Retention insert gray, ZERO RETENTION	30001-01	30001-01	30001-01	30001-01	-
	Locator R-Tx® Retention insert blue, LIGHT	30002-01	30002-01	30002-01	30002-01	-
	Locator R-Tx® Retention insert pink, MEDIUM	30003-01	30003-01	30003-01	30003-01	-
	Locator R-Tx® Retention insert white, STRONG	30004-01	30004-01	30004-01	30004-01	-

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Locator® Abutment	C2253.3310	C2253.3810	C2253.4310	C2253.5010	1.0 mm
		C2253.3320	C2253.3820	C2253.4320	C2253.5020	2.0 mm
		C2253.3330	C2253.3830	C2253.4330	C2253.5030	3.0 mm
		C2253.3340	C2253.3840	C2253.4340	C2253.5040	4.0 mm
		-	C2253.3850	C2253.4350	C2253.5050	5.0 mm
	Locator® Impression cap	J2253.0200	J2253.0200	J2253.0200	J2253.0200	-
	Locator® Analog	J2253.0340	J2253.0340	J2253.0340	J2253.0340	-
	Locator® Male processing package	J2253.0102	J2253.0102	J2253.0102	J2253.0102	-
	Locator® Male processing package for extended range	-	J2253.0112	J2253.0112	J2253.0112	-
	CONELOG® Universal abutment	-	C2211.3800	C2211.4300	C2211.5000	-
	CONELOG® Telescope abutment	-	C2212.3800	C2212.4300	C2212.5000	-

CAD/CAM prosthetics






	CONELOG® Scanbodies	C2600.3310	C2600.4310	C2600.4310	C2600.5010	-
	CONELOG® ScanPost for Sirona® Scanbody	C2620.3306	C2620.3806	C2620.4306	C2620.5006	-
	CONELOG® CAM titanium blank, type IAC	C2411.3313	C2411.4313	C2411.4313	C2411.5013	-
	CONELOG® CAM titanium blank, type ME	C2421.3320	C2421.3820	C2421.4320	C2421.5020	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-

DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

Screw overview Abutment and prosthetic screws – intraoral use

Implant-Abutment connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm						
		M 1.6			M 2.0						
Article	CONELOG® Abutment screw					Tightening torque					
	Scanbody ScanPost for Sirona® Scanbody	8.9 mm  C4005.1601			8.9 mm  C4005.2001		tightened by hand**				
	Temporary abutments titanium, crown and bridge										
	Esthomic® Abutments										
	Universal abutment										20 Ncm*
	Telescope abutment										
	Gold-plastic abutment										
	Logfit® Abutment										
	Vario SR abutments, 20° und 30° angled										
	CONELOG® CAM titanium blank, type IAC and ME										
		CONELOG® Abutment screws for titanium bases CAD/CAM, dark purple anodized									
	Titanium bases CAD/CAM, crown and bridge	8.9 mm  C4015.1601			8.9 mm  C4015.2001		20 Ncm*				
		CONELOG® Vario SR abutment screws									
	Vario SR abutment, straight	10.6 mm  C4007.1600			10.6 mm  C4007.2000		20 Ncm*				
		CONELOG® Abutment screws with reduced head, light blue anodized									
	COMFOUR® Bar abutments, 17° and 30° angled	7.8 mm  C4004.1601			7.8 mm  C4004.2001		20 Ncm*				

* with torque wrench J5320.1030

** Optional for temporary abutments titanium: torque after completed healing phase 20 Ncm.



All screws must be retightened with the corresponding torque after at least 5 minutes!

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		M 1.6			M 2.0	
Article		Prosthetic screws for bar abutments, light blue anodized				Tightening torque
	COMFOUR® Bar abutments, 17° and 30° angled	3.6 mm  J4012.1601			3.8 mm  J4012.2001	15 Ncm*
		Vario SR prosthetic screw, yellow anodized				
	Vario SR abutments, straight, 20° and 30° angled	4 mm  J4005.2004				15 Ncm*

Auxiliary screws Intra- and extraoral use

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm		
		M 1.6			M 2.0		
Article		Prosthetic screws for bar abutments, light blue anodized				Tightening torque	
	Scanning cap for bar abutments	3.6 mm  J4012.1601		3.8 mm  J4012.2001		tightened by hand	
		Screws for bar abutments, for impression taking open tray and for soldering, light blue anodized					
	COMFOUR® Bar abutments, straight, 17° and 30° angled	12 mm  J4012.1610		12.2 mm  J4012.2010		tightened by hand	
		17 mm  J4012.1615		17.2 mm  J4012.2015			
		22 mm  J4012.1620		22.2 mm  J4012.2020			
		Plastic screws for bar abutment, as fixation and bonding aid, beige					
		29 mm  J4009.1627		29.2 mm  J4009.2027			tightened by hand

* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

Screw overview Lab screws – extraoral use

Lab analog-Abutment connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M 1.6			M 2.0	
Article	CONELOG® Lab screws*, brown anodized				Tightening torque
 Scanbody ScanPost for Sirona® Scanbody	 8.9 mm C4006.1601			 8.9 mm C4006.2001	tightened by hand
 Temporary abutments titanium, crown and bridge					
 Esthomic® Abutments					
 Universal abutment Telescope abutment Gold-plastic abutment					
 Vario SR abutments, 20° and 30° angled					
 CONELOG® CAM titanium blank, type IAC and ME					
CONELOG® Lab screws for titanium bases CAD/CAM*, brown anodized					
 Titanium bases CAD/CAM, crown and bridge	 8.9 mm C4016.1601			 8.9 mm C4016.2001	tightened by hand
CONELOG® Bonding aids**					
 Titanium bases CAD/CAM, crown and bridge	 26 mm			 26 mm	tightened by hand
CONELOG® Vario SR lab screws*, brown anodized					
 Vario SR abutment, straight	 10.6 mm C4008.1600			 10.6 mm C4008.2000	tightened by hand
CONELOG® Lab screws with reduced head*, light blue partially anodized					
 COMFOUR® Bar abutments, 17° and 30° angled	 7.8 mm C4004.1600			 7.8 mm C4004.2000	tightened by hand

* Lab screws may not be used on patients.

** not available singly, are included in the packaging of the titanium base CAD/CAM.

Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm		
		M 1.6			M 2.0		
Article		Lab prosthetic screws for bar abutments*, brown anodized				Tightening torque	
	Scanning cap for bar abutments	3.6 mm  J4013.1601			3.8 mm  J4013.2001		tightened by hand
	COMFOUR® Bar abutment, 17° and 30° angled						
	Bar lab analog for bar abutments						
		Vario SR prosthetic screw, yellow anodized					
	Vario SR abutments, straight, 20° and 30° angled	4 mm  J4005.2004				tightened by hand	
	Vario SR analog						
		Prosthetic screw for bar abutments*, for fabrication of the wax up on the bar sleeve for titanium bonding base, Passive-Fit, on the bar lab analog					
	Titanium bonding base for bar abutments and bar sleeve for titanium bonding base, burn-out, Passive-Fit	5.5 mm  J4005.1602			5.5 mm  J4005.2002		tightened by hand

* Lab screws may not be used on patients.

Overview Tightening torque

Article	Instrument	Tightening torque
 Implant cover screw		tightened by hand**
 Healing caps cylindrical, wide body, bottleneck		
 Impression posts Bite registration post		
 Lab screws		
 Lab screws with reduced head		
 Temporary abutments titanium, crown and bridge	 J5317.0510  J5317.0501  J5317.0502  J5317.0504  J5317.0503	20 Ncm*
 Abutment screws		
 Abutment screws with reduced head		
 Esthomic® Abutment, straight		
 Esthomic® Abutment, angled 15°/20°		
 Esthomic® Abutment, Inset		
 Universal abutment		
 Telescope abutment		
 Gold-plastic abutment		
 Logfit® Abutments		
 Titanium bases CAD/CAM, crown and bridge		
 CONELOG® CAM titanium blank, type IAC and ME		

* with the torque wrench J5320.1030

** Optional for temporary abutments titanium: torque after completed healing phase 20 Ncm.

All screws must be retightened with the corresponding torque after at least 5 minutes!

		3.3 mm	3.8 mm	4.3 mm	Ø 5.0 mm	3.3	3.8	4.3	5.0	6.0		
Article		Instrument				Tightening torque						
	Bar abutment, straight	 J5300.0020		 J5300.0021	 J5300.0025	20 Ncm*	30 Ncm*					
	Bar abutment, 17° and 30° angled	 J5317.0510				20 Ncm*						
	Scanning cap for bar abutments					tightened by hand						
	Titanium cap for bar abutment, for crown/bridge					15 Ncm*						
	Crown base for bar abutment, burn-out											
	Bases for bar abutments burn-out, cast-on, solderable, laser-weldable											
	Titanium bonding bases for bar abutment, Passive-Fit											
	Locator R-Tx® Abutment					 J5317.0504		 J5317.0503	20 Ncm*	30 Ncm*		
	Healing cap for bar abutment					 J5300.0027				tightened by hand		
	Impression cap for bar abutment, closed tray (bridge/bar)	 J5300.0028										
	Ball abutments	 J5300.0011				20 Ncm*	30 Ncm*					
	Locator® Abutments	 J2253.0001				20 Ncm*						
	Locator® Fixture for bar abutment											
	Scanbodies	 J5317.0501				tightened by hand						
	ScanPosts for Sirona® Scanbody									 J5317.0502		

* with the torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

Materials

Titanium Grade 4		
Properties (ASTM F67)		
Chemical structure (in %)	O	≤ 0.4
	Fe	≤ 0.5
	C	≤ 0.08
	N	≤ 0.05
	H	≤ 0.015
	Ti	Rest
Mechanical properties	Tensile strength	≥ 550 MPa
	Elongation at break	≥ 12 %

Titanium alloy Ti6Al4V ELI		
Properties (ASTM F136)		
Chemical structure (in %)	Al	5.5 – 6.5
	V	3.5 – 4.5
	Fe	≤ 0.25
	C	≤ 0.08
	N	≤ 0.05
	O	≤ 0.13
	H	≤ 0.012
	Ti	Rest
Mechanical properties	Tensile strength	≥ 860 MPa
	Elongation at break	≥ 10 %

Cast-on gold alloy CONELOG® Gold-plastic abutment		
Properties		
Chemical structure (in %)	Au	60
	Pd	20
	Pt	19
	Ir	1
Physical properties	Melting range	1400 – 1490 °C
	Density	17.5 g/cm³
	E-Modul	136 GPa
	Coefficient of thermal expansion (25 – 500°C)	11.9 µm/m· °C
	Coefficient of thermal expansion (25 – 600°C)	12.2 µm/m· °C
	Color	white
Mechanical properties	drawn	
	Hardness HV5	> 215
	Tensile strength (Rm)	> 750 MPa
	0.2% Elongation limit (Rp 0.2%)	> 650 MPa
	Elongation at break	> 2 %

Cast-on gold alloy base for bar abutment		
Properties		
Chemical structure (in %)	Au	60
	Pt	19
	Pd	20
	Ir	1
Physical properties	Density	17.5 g/cm³
	Color	white
	Liquidus	1490 °C
	Solidus	1400 °C
	Coefficient of thermal expansion (25 – 500°C)	12.5 µm/m· °C
	Coefficient of thermal expansion (25 – 600°C)	12.6 µm/m· °C
	E-Modul	136 GPa
Mechanical properties	hardened 700 °C/30 min.	
	Hardness HV5	210
	0.2 % Elongation limit	450 – 570 MPa
	Elongation at break	min. 10 %
	Tensile strength MPa	530 – 650

Solderable gold alloy base for bar abutment

Properties

Chemical structure (in %)	Au	68.60
	Pt	2.45
	Ag	11.85
	Pd	3.95
	Cu	10.60
	Zn	2.50
	Ir	0.05
	Rh	-
	Ru	-
Physical properties	Color	yellow
	Melting range	880 – 940 °C
Mechanical properties	Hardness	
	annealed HV5	175
	hardened HV5	275
	self hardened HV5	240

A		C	
Abutment collets	82	CAM titanium blank	64
Abutment screw for CONELOG® Titanium bases CAD/CAM	63	Cardanic driver	46
Abutment screw, hex	70, 77	Cleaning cannula	48
Adapter for screw implants	47	Cleaning needle	48
Adapter ISO shaft for angled hand piece	46	Collet for CAM blank, type IAC	64
Aligning tool	68	COMFOUR® Patient brochure	88
ALTApin applicator	53	Countersink	43
ALTApin magazine	55	Crown base for bar abutment	69
ALTApin membrane fixator	54	CT-tube	17
ALTApin pricker	54		
ALTApin pricker, insert	54	D	
ALTApin set	53	Demonstration model, acrylic glass	87
ALTApin single patient drill, ISO shaft	54	Dense bone drill PROGRESSIVE-LINE	23
ALTApin surgery mallet	54	Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE	23, 37
ALTApin tray	53	Depth stop SCREW-LINE	43
Appointment pad	89	DIM Analog® for the CONELOG® Implant System	59
		Disconnecter	81
B		Drill extension ISO shaft, for instruments with internal irrigation not for instruments with internal irrigation	41 44
Ball abutment analogs	72	Drill for CT-tube	17
Ball abutments, male part	71	Drill PROGRESSIVE-LINE Flex	27
Bar abutment	67	Driver for ball abutment	78
Bar implant analog for bar abutments	68	Driver for impression cap and healing cap for bar abutment	68, 79
Bar lab analog for bar abutments	68	Driver for Locator®	79
Bar sleeve for titanium bonding base	69	Driver for screw implants	45
Baring drill for cover screw	43	Driver for straight bar abutment	78, 79
Base for bar abutment	69		
Bite registration caps	59	E	
Bite registration posts	59	Edentulous mandible	87
Bone profiler	43		

E		G	
Esthomic® Abutments	60, 61	Guide System surgery set, SCREW-LINE	39
Esthomic® Abutments, Inset	61	Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30
Esthomic® Selection abutments	83	Guide System template drill	40
F		Guide System template drill PROGRESSIVE-LINE	32
Form drill PROGRESSIVE-LINE	23	Guiding pin for bone profiler	43
Form drill SCREW-LINE	37	H	
Form drill SCREW-LINE Cortical bone	37	Handle for CAMLOG®/CONELOG® Implant analog	81
G		Healing cap for bar abutment	68
Gingiva height indicator, straight	68	Healing cap	55
Gold-plastic abutment	65	Holding key for insertion post	47
Guide System check-up pin	41	Holding sleeve for screw implants	47
Guide System check-up pin PROGRESSIVE-LINE	32	I	
Guide System dense bone drill PROGRESSIVE-LINE	31	Implant analog	59
Guide System driver	41	Implant cover screw	55
Guide System form drill PROGRESSIVE-LINE	31	Implant pass	88
Guide System form drill for Ø 3.8 mm under preparation PROGRESSIVE-LINE	31	Impression cap for bar abutment, closed tray	68
Guide System form drill SCREW-LINE, Cortical bone	39	Impression caps for impression post, closed tray	58
Guide System gingiva punch	39	Impression posts	58
Guide System gingiva punch PROGRESSIVE-LINE	30	L	
Guide System guiding sleeve	40	Lab analog	59
Guide System guiding sleeve PROGRESSIVE-LINE	32	Lab prosthetic screw for bar abutment, hex	70
Guide System Insertion post, screw-mounted	32, 40	Lab screw for CONELOG® Titanium bases CAD/CAM	63
Guide System pilot drill PROGRESSIVE-LINE	30	Lab screw, hex	70, 77
Guide System pilot drill set	38	Lamella retention insert	71
Guide System pre-drill PROGRESSIVE-LINE	31	Locator® Abutment	74
Guide System seating tool	40	Locator® Abutment holder sleeve	79
Guide System setting tool PROGRESSIVE-LINE	32		

L		M	
Locator® Analog	74	Manual screwdriver, hex	48, 81
Locator® Angle measurement guide	79	Matrix CM Dalbo®-Plus	71
Locator® Block out spacer	75	Modeling aids for CAMLOG® Titanium bases CAD/CAM	63
Locator® Fixture for bar abutment	70		
Locator® Impression cap	74	O	
Locator® Instrument	79	Orientation gauge for COMFOUR®	68
Locator® Male processing package	75	Osteotome SCREW-LINE	49, 50, 51, 52
Locator® Male processing package for extended range	75	Osteotomy set CAMLOG®/CONELOG® SCREW-LINE	49, 50, 51, 52
Locator® Parallel post	79		
Locator® Processing replacement male	75	P	
Locator® Replacement male	75, 76	Paralleling pin PROGRESSIVE-LINE	23
Locator® Replacement male for extended range	76	Paralleling pin SCREW-LINE	44
Locator R-Tx® Abutment	72	Patient advice sheets	88
Locator R-Tx® Analog	72, 73	Patient brochure	88
Locator R-Tx® Impression coping	72	Pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE CAMLOG®/CONELOG® SCREW-LINE	22 36
Locator R-Tx® Retention insert	73, 74	PickUp instrument	46
Locator R-Tx® Retention insert tool	80	Pilot drill	42
Locator R-Tx® Processing insert	73	Pilot drill SCREW-LINE	42
Locator R-Tx® Processing spacer	73	Plastic screw for bar abutment	71
Locator R-Tx® Titanium housing	73	Point drill	42
Logfit® Abutments	66	Polishing protection for caps and bases for bar abutment	69
Logfit® Analog	66	Poster	89
Logfit® Impression caps	66	Pre-drill SCREW-LINE	42
Logfit® Plastic copings (without rotation securing device)	66	Pre-Osteotome SCREW-LINE	49, 50, 51, 52
		Presentation folder	88
		Profile drill PROGRESSIVE-LINE Flex	27
		PROGRESSIVE-LINE Implant for practice	86

P		T	
PROGRESSIVE-LINE Implant, Promote® plus	19	Tap adapter	44
PROGRESSIVE-LINE Macro model	87	Tap PROGRESSIVE-LINE	23
Prosthetic screw for bar abutments	70	Tap SCREW-LINE	37
Prosthetic set	80	Telescope abutments, for double crown restorations	77
Prosthetic tray	80	Temporary abutment, titanium alloy	60
Prosthetic tray universal	80	Titanium bases CAD/CAM	62
R		Titanium bonding base for bar abutment	69
Removal adapter for CAMLOG® and CONELOG®	23	Titanium cap for bar abutment	68, 69
Reworking reamer, for base for bar abutment	82	Titanium cap without retention for bar abutment, for bridge	69
Round bur	42	Torque wrench	78
S		U	
Scanbodies	63	Universal abutments	65
Scanning cap for bar abutments	68	Universal abutments, for double crown restorations	77
ScanPosts for Sirona® Scanbody	63	Universal holder	82
Screw, hex	70	W	
Screwdriver Activator	78	Wrench adapter	27
Screwdriver, hex	47, 48, 80, 81	X	
SCREW-LINE Implant for practice	86	X-Ray Planning foil 1.25:1 CONELOG® PROGRESSIVE-LINE Implants	16
SCREW-LINE Implant, Promote® plus	33	CONELOG® SCREW-LINE Implants	16
SCREW-LINE Macro model	87	X-Ray Planning foil 1.4:1 CONELOG® PROGRESSIVE-LINE Implants	16
Selection abutment kit	83	CONELOG® SCREW-LINE Implants	16
Surgery set		X-Ray Transfer pictures 1.25:1 CONELOG® SCREW-LINE Implants	16
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22		
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	26		
CAMLOG®/CONELOG® SCREW-LINE	36		
Surgery tray			
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22		
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	26		
CAMLOG®/CONELOG® SCREW-LINE	36		
Surgery wash tray			
CAMLOG®/CONELOG® PROGRESSIVE-LINE	22		
CAMLOG®/CONELOG® SCREW-LINE	36		

05003503	Matrix CM Dalbo®-Plus	71	B1012	Point drill	42
05003504	Lamella retention insert	71		SCREW-LINE Implant, Promote® plus incl. screw-mounted insertion post	
07000389	Screwdriver Activator	78	C1065.3309	Ø 3.3 mm, L 9 mm	33
			C1065.3311	Ø 3.3 mm, L 11 mm	33
08394	Locator® Abutment holder sleeve	79	C1065.3313	Ø 3.3 mm, L 13 mm	33
			C1065.3316	Ø 3.3 mm, L 16 mm	33
	Locator® R-Tx™ Retention insert		C1065.3807	Ø 3.8 mm, L 7 mm	33
30001-01	Ø 3.3/3.8/4.3/5.0 mm, gray	73	C1065.3809	Ø 3.8 mm, L 9 mm	33
30002-01	Ø 3.3/3.8/4.3/5.0 mm, blue	73	C1065.3811	Ø 3.8 mm, L 11 mm	33
30003-01	Ø 3.3/3.8/4.3/5.0 mm, pink	73	C1065.3813	Ø 3.8 mm, L 13 mm	33
30004-01	Ø 3.3/3.8/4.3/5.0 mm, white	74	C1065.3816	Ø 3.8 mm, L 16 mm	33
			C1065.4307	Ø 4.3 mm, L 7 mm	33
	Locator® R-Tx™ Processing insert		C1065.4309	Ø 4.3 mm, L 9 mm	33
30012-01	Ø 3.3/3.8/4.3/5.0 mm	73	C1065.4311	Ø 4.3 mm, L 11 mm	33
			C1065.4313	Ø 4.3 mm, L 13 mm	33
	Locator® R-Tx™ Titanium housing		C1065.4316	Ø 4.3 mm, L 16 mm	33
30013-01	Ø 3.3/3.8/4.3/5.0 mm	73	C1065.5007	Ø 5.0 mm, L 7 mm	33
			C1065.5009	Ø 5.0 mm, L 9 mm	33
	Locator® R-Tx™ Analog		C1065.5011	Ø 5.0 mm, L 11 mm	33
30014-01	Ø 3.3/3.8/4.3 mm	72	C1065.5013	Ø 5.0 mm, L 13 mm	33
30016-01	Ø 5.0 mm	73	C1065.5016	Ø 5.0 mm, L 16 mm	33
				SCREW-LINE Implant, Promote® plus incl. snap-in insertion post	
30017-01	Locator® R-Tx™ Impression coping Ø 3.3/3.8/4.3/5.0 mm	72	C1066.3309	Ø 3.3 mm, L 9 mm	33
			C1066.3311	Ø 3.3 mm, L 11 mm	33
30018-01	Locator® R-Tx™ Processing spacer Ø 3.3/3.8/4.3/5.0 mm	73	C1066.3313	Ø 3.3 mm, L 13 mm	33
			C1066.3316	Ø 3.3 mm, L 16 mm	33
30021-01	Locator® R-Tx™ Retention insert tool	80	C1066.3807	Ø 3.8 mm, L 7 mm	33
			C1066.3809	Ø 3.8 mm, L 9 mm	33
	Locator® R-Tx™ Abutment		C1066.3811	Ø 3.8 mm, L 11 mm	33
30805-01	Ø 3.3 mm, GH 1.0 mm	72	C1066.3813	Ø 3.8 mm, L 13 mm	33
30805-02	Ø 3.3 mm, GH 2.0 mm	72	C1066.3816	Ø 3.8 mm, L 16 mm	33
30805-03	Ø 3.3 mm, GH 3.0 mm	72	C1066.4307	Ø 4.3 mm, L 7 mm	33
30805-04	Ø 3.3 mm, GH 4.0 mm	72	C1066.4309	Ø 4.3 mm, L 9 mm	33
30806-01	Ø 3.8 mm, GH 1.0 mm	72	C1066.4311	Ø 4.3 mm, L 11 mm	33
30806-02	Ø 3.8 mm, GH 2.0 mm	72	C1066.4313	Ø 4.3 mm, L 13 mm	33
30806-03	Ø 3.8 mm, GH 3.0 mm	72	C1066.4316	Ø 4.3 mm, L 16 mm	33
30806-04	Ø 3.8 mm, GH 4.0 mm	72	C1066.5007	Ø 5.0 mm, L 7 mm	33
30806-05	Ø 3.8 mm, GH 5.0 mm	72	C1066.5009	Ø 5.0 mm, L 9 mm	33
30807-01	Ø 4.3 mm, GH 1.0 mm	72	C1066.5011	Ø 5.0 mm, L 11 mm	33
30807-02	Ø 4.3 mm, GH 2.0 mm	72	C1066.5013	Ø 5.0 mm, L 13 mm	33
30807-03	Ø 4.3 mm, GH 3.0 mm	72	C1066.5016	Ø 5.0 mm, L 16 mm	33
30807-04	Ø 4.3 mm, GH 4.0 mm	72			
30807-05	Ø 4.3 mm, GH 5.0 mm	72			
30808-01	Ø 5.0 mm, GH 1.0 mm	72	C1069.3813	Ø 3.8 mm	86
30808-02	Ø 5.0 mm, GH 2.0 mm	72	C1069.4313	Ø 4.3 mm	86
30808-03	Ø 5.0 mm, GH 3.0 mm	72			
30808-04	Ø 5.0 mm, GH 4.0 mm	72			
30808-05	Ø 5.0 mm, GH 5.0 mm	72			
				PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post	
			C1085.3309	Ø 3.3 mm, L 9 mm	19
A2002.2000	CT-tube	17	C1085.3311	Ø 3.3 mm, L 11 mm	19
			C1085.3313	Ø 3.3 mm, L 13 mm	19
	Drill for CT-tube		C1085.3316	Ø 3.3 mm, L 16 mm	19
A2050.2600	Ø 2.6 mm	17	C1085.3807	Ø 3.8 mm, L 7 mm	19
A2050.2800	Ø 2.8 mm	17	C1085.3809	Ø 3.8 mm, L 9 mm	19
			C1085.3811	Ø 3.8 mm, L 11 mm	19
A2222.2200	CT-tube	17	C1085.3813	Ø 3.8 mm, L 13 mm	19

	PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post			Healing cap, cylindrical	
C1085.3816	Ø 3.8 mm, L 16 mm	19	C2015.3820	Ø 3.8 mm, GH 2.0 mm	55
C1085.4307	Ø 4.3 mm, L 7 mm	19	C2015.3840	Ø 3.8 mm, GH 4.0 mm	55
C1085.4309	Ø 4.3 mm, L 9 mm	19	C2015.3860	Ø 3.8 mm, GH 6.0 mm	55
C1085.4311	Ø 4.3 mm, L 11 mm	19	C2015.4320	Ø 4.3 mm, GH 2.0 mm	55
C1085.4313	Ø 4.3 mm, L 13 mm	19	C2015.4340	Ø 4.3 mm, GH 4.0 mm	55
C1085.4316	Ø 4.3 mm, L 16 mm	19	C2015.4360	Ø 4.3 mm, GH 6.0 mm	55
C1085.5007	Ø 5.0 mm, L 7 mm	19	C2015.5020	Ø 5.0 mm, GH 2.0 mm	55
C1085.5009	Ø 5.0 mm, L 9 mm	19	C2015.5040	Ø 5.0 mm, GH 4.0 mm	55
C1085.5011	Ø 5.0 mm, L 11 mm	19	C2015.5060	Ø 5.0 mm, GH 6.0 mm	55
C1085.5013	Ø 5.0 mm, L 13 mm	19		Implant cover screw	
C1085.5016	Ø 5.0 mm, L 16 mm	19	C2019.3300	Ø 3.3 mm	55
	PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post		C2019.3800	Ø 3.8 mm	55
C1086.3309	Ø 3.3 mm, L 9 mm	19	C2019.4300	Ø 4.3 mm	55
C1086.3311	Ø 3.3 mm, L 11 mm	19	C2019.5000	Ø 5.0 mm	55
C1086.3313	Ø 3.3 mm, L 13 mm	19		Guide System CONELOG® Insertion post	
C1086.3316	Ø 3.3 mm, L 16 mm	19	C2026.3303	Ø 3.3 mm	32, 40
C1086.3807	Ø 3.8 mm, L 7 mm	19	C2026.3803	Ø 3.8 mm	32, 40
C1086.3809	Ø 3.8 mm, L 9 mm	19	C2026.4303	Ø 4.3 mm	32, 40
C1086.3811	Ø 3.8 mm, L 11 mm	19	C2026.5003	Ø 5.0 mm	32
C1086.3813	Ø 3.8 mm, L 13 mm	19		Impression post, closed tray	
C1086.3816	Ø 3.8 mm, L 16 mm	19	C2110.3300	Ø 3.3 mm	58
C1086.4307	Ø 4.3 mm, L 7 mm	19	C2110.3800	Ø 3.8 mm	58
C1086.4309	Ø 4.3 mm, L 9 mm	19	C2110.4300	Ø 4.3 mm	58
C1086.4311	Ø 4.3 mm, L 11 mm	19	C2110.5000	Ø 5.0 mm	58
C1086.4313	Ø 4.3 mm, L 13 mm	19		Impression post, open tray	
C1086.4316	Ø 4.3 mm, L 16 mm	19	C2121.3300	Ø 3.3 mm	58
C1086.5007	Ø 5.0 mm, L 7 mm	19	C2121.3800	Ø 3.8 mm	58
C1086.5009	Ø 5.0 mm, L 9 mm	19	C2121.4300	Ø 4.3 mm	58
C1086.5011	Ø 5.0 mm, L 11 mm	19	C2121.5000	Ø 5.0 mm	58
C1086.5013	Ø 5.0 mm, L 13 mm	19		Bite registration posts	
C1086.5016	Ø 5.0 mm, L 16 mm	19	C2140.3300	Ø 3.3 mm	59
	PROGRESSIVE-LINE Implant for practice		C2140.3800	Ø 3.8 mm	59
C1901.3813	Ø 3.8 mm	86	C2140.4300	Ø 4.3 mm	59
C1901.4313	Ø 4.3 mm	86	C2140.5000	Ø 5.0 mm	59
	Healing cap, bottleneck			Universal abutments	
C2011.3340	Ø 3.3 mm, GH 4.0 mm	55	C2211.3300	Ø 3.3 mm	65
C2011.3840	Ø 3.8 mm, GH 4.0 mm	55	C2211.3800	Ø 3.8 mm	65, 77
C2011.3860	Ø 3.8 mm, GH 6.0 mm	55	C2211.4300	Ø 4.3 mm	65, 77
C2011.4340	Ø 4.3 mm, GH 4.0 mm	55	C2211.5000	Ø 5.0 mm	65, 77
C2011.4360	Ø 4.3 mm, GH 6.0 mm	55		Telescope abutment for double crown restorations	
C2011.5040	Ø 5.0 mm, GH 4.0 mm	55	C2212.3800	Ø 3.8 mm	77
C2011.5060	Ø 5.0 mm, GH 6.0 mm	55	C2212.4300	Ø 4.3 mm	77
	Healing cap, wide body		C2212.5000	Ø 5.0 mm	77
C2014.3340	Ø 3.3 mm, GH 4.0 mm	55		Esthomic® Abutments, straight	
C2014.3840	Ø 3.8 mm, GH 4.0 mm	55	C2226.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	60
C2014.3860	Ø 3.8 mm, GH 6.0 mm	55	C2226.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	60
C2014.4340	Ø 4.3 mm, GH 4.0 mm	55	C2226.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	60
C2014.4360	Ø 4.3 mm, GH 6.0 mm	55	C2226.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	60
C2014.5040	Ø 5.0 mm, GH 4.0 mm	55	C2226.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	60
C2014.5060	Ø 5.0 mm, GH 6.0 mm	55	C2226.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	60
	Healing cap, cylindrical				
C2015.3320	Ø 3.3 mm, GH 2.0 mm	55			
C2015.3340	Ø 3.3 mm, GH 4.0 mm	55			

Esthomic® Abutments, 15° angled, type A			Titanium bases CAD/CAM, crown		
C2227.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	60	C2242.3820	Ø 3.8 mm, GH 2.0 mm	62
C2227.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	60	C2242.4308	Ø 4.3 mm, GH 0.8 mm	62
C2227.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	60	C2242.4320	Ø 4.3 mm, GH 2.0 mm	62
C2227.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	60	C2242.5008	Ø 5.0 mm, GH 0.8 mm	62
C2227.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	60	C2242.5020	Ø 5.0 mm, GH 2.0 mm	62
C2227.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	60	Gold-plastic abutment		
Esthomic® Abutments, 15° angled, type B			C2246.3300	Ø 3.3 mm	65
C2228.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	61	C2246.3800	Ø 3.8 mm	65
C2228.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	61	C2246.4300	Ø 4.3 mm	65
C2228.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	61	C2246.5000	Ø 5.0 mm	65
C2228.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	61	Ball abutments, male part		
C2228.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	61	C2249.3315	Ø 3.3 mm, GH 1.5 mm	71
C2228.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	61	C2249.3330	Ø 3.3 mm, GH 3.0 mm	71
Esthomic® Abutments, 20° angled, type A			C2249.3815	Ø 3.8 mm, GH 1.5 mm	71
C2231.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	61	C2249.3830	Ø 3.8 mm, GH 3.0 mm	71
C2231.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	61	C2249.3845	Ø 3.8 mm, GH 4.5 mm	71
C2231.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	61	C2249.4315	Ø 4.3 mm, GH 1.5 mm	71
C2231.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	61	C2249.4330	Ø 4.3 mm, GH 3.0 mm	71
C2231.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	61	C2249.4345	Ø 4.3 mm, GH 4.5 mm	71
C2231.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	61	C2249.5015	Ø 5.0 mm, GH 1.5 mm	71
Esthomic® Abutments, 20° angled, type B			C2249.5030	Ø 5.0 mm, GH 3.0 mm	71
C2232.3815	Ø 3.8 mm, GH 1.5 – 2.5 mm	61	C2249.5045	Ø 5.0 mm, GH 4.5 mm	71
C2232.3830	Ø 3.8 mm, GH 3.0 – 4.5 mm	61	Locator® Abutments		
C2232.4315	Ø 4.3 mm, GH 1.5 – 2.5 mm	61	C2253.3310	Ø 3.3 mm, GH 1.0 mm	74
C2232.4330	Ø 4.3 mm, GH 3.0 – 4.5 mm	61	C2253.3320	Ø 3.3 mm, GH 2.0 mm	74
C2232.5015	Ø 5.0 mm, GH 1.5 – 2.5 mm	61	C2253.3330	Ø 3.3 mm, GH 3.0 mm	74
C2232.5030	Ø 5.0 mm, GH 3.0 – 4.5 mm	61	C2253.3340	Ø 3.3 mm, GH 4.0 mm	74
Esthomic® Abutments, Inset			C2253.3810	Ø 3.8 mm, GH 1.0 mm	74
C2235.3320	Ø 3.3 mm, GH 2.0 – 3.3 mm	61	C2253.3820	Ø 3.8 mm, GH 2.0 mm	74
C2235.3820	Ø 3.8 mm, GH 2.0 – 3.3 mm	61	C2253.3830	Ø 3.8 mm, GH 3.0 mm	74
C2235.4320	Ø 4.3 mm, GH 2.0 – 3.3 mm	61	C2253.3840	Ø 3.8 mm, GH 4.0 mm	74
C2235.5020	Ø 5.0 mm, GH 2.0 – 3.3 mm	61	C2253.3850	Ø 3.8 mm, GH 5.0 mm	74
Temporary abutment, crown			C2253.4310	Ø 4.3 mm, GH 1.0 mm	74
C2239.3300	Ø 3.3 mm	60	C2253.4320	Ø 4.3 mm, GH 2.0 mm	74
C2239.3800	Ø 3.8 mm	60	C2253.4330	Ø 4.3 mm, GH 3.0 mm	74
C2239.4300	Ø 4.3 mm	60	C2253.4340	Ø 4.3 mm, GH 4.0 mm	74
C2239.5000	Ø 5.0 mm	60	C2253.4350	Ø 4.3 mm, GH 5.0 mm	74
Modeling aids for CONELOG®			C2253.5010	Ø 5.0 mm, GH 1.0 mm	74
Titanium bases CAD/CAM			C2253.5020	Ø 5.0 mm, GH 2.0 mm	74
C2242.3302	Ø 3.3 mm	63	C2253.5030	Ø 5.0 mm, GH 3.0 mm	74
C2242.3802	Ø 3.8 mm	63	C2253.5040	Ø 5.0 mm, GH 4.0 mm	74
C2242.4302	Ø 4.3 mm	63	C2253.5050	Ø 5.0 mm, GH 5.0 mm	74
C2242.5002	Ø 5.0 mm	63	Bar abutments, straight		
Titanium bases CAD/CAM, crown			C2254.3310	Ø 3.3 mm, GH 1.0 mm	67
C2242.3308	Ø 3.3 mm, GH 0.8 mm	62	C2254.3325	Ø 3.3 mm, GH 2.5 mm	67
C2242.3320	Ø 3.3 mm, GH 2.0 mm	62	C2254.3810	Ø 3.8 mm, GH 1.0 mm	67
C2242.3808	Ø 3.8 mm, GH 0.8 mm	62	C2254.3825	Ø 3.8 mm, GH 2.5 mm	67
			C2254.3840	Ø 3.8 mm, GH 4.0 mm	67
			C2254.4310	Ø 4.3 mm, GH 1.0 mm	67
			C2254.4325	Ø 4.3 mm, GH 2.5 mm	67
			C2254.4340	Ø 4.3 mm, GH 4.0 mm	67
			C2254.5010	Ø 5.0 mm, GH 1.0 mm	67
			C2254.5025	Ø 5.0 mm, GH 2.5 mm	67
			C2254.5040	Ø 5.0 mm, GH 4.0 mm	67

Bar abutments, 17° angled, type A			CAM titanium blank, type ME		
C2256.3325	Ø 3.3 mm, GH 2.5 mm	67	C2421.3320	Ø 3.3 mm	64
C2256.3340	Ø 3.3 mm, GH 4.0 mm	67	C2421.3820	Ø 3.8 mm	64
C2256.3825	Ø 3.8 mm, GH 2.5 mm	67	C2421.4320	Ø 4.3 mm	64
C2256.3840	Ø 3.8 mm, GH 4.0 mm	67	C2421.5020	Ø 5.0 mm	64
C2256.4325	Ø 4.3 mm, GH 2.5 mm	67			
C2256.4340	Ø 4.3 mm, GH 4.0 mm	67		Logfit® Abutments	
C2256.5025	Ø 5.0 mm, GH 2.5 mm	67	C2550.3810	Ø 3.8 mm, GH 1.0 mm	66
C2256.5040	Ø 5.0 mm, GH 4.0 mm	67	C2550.3825	Ø 3.8 mm, GH 2.5 mm	66
			C2550.4310	Ø 4.3 mm, GH 1.0 mm	66
Bar abutments, 17° angled, type B			C2550.4325	Ø 4.3 mm, GH 2.5 mm	66
C2257.3325	Ø 3.3 mm, GH 2.5 mm	67	C2550.5010	Ø 5.0 mm, GH 1.0 mm	66
C2257.3340	Ø 3.3 mm, GH 4.0 mm	67	C2550.5025	Ø 5.0 mm, GH 2.5 mm	66
C2257.3825	Ø 3.8 mm, GH 2.5 mm	67			
C2257.3840	Ø 3.8 mm, GH 4.0 mm	67		Scanbodies	
C2257.4325	Ø 4.3 mm, GH 2.5 mm	67	C2600.3310	Ø 3.3 mm	63
C2257.4340	Ø 4.3 mm, GH 4.0 mm	67	C2600.4310	Ø 3.8/4.3 mm	63
C2257.5025	Ø 5.0 mm, GH 2.5 mm	67	C2600.5010	Ø 5.0 mm	63
C2257.5040	Ø 5.0 mm, GH 4.0 mm	67			
				ScanPosts for Sirona® Scanbody	
Bar abutments, 30° angled, type A			C2620.3306	Ø 3.3 mm	63
C2258.3325	Ø 3.3 mm, GH 2.5 mm	67	C2620.3806	Ø 3.8 mm	63
C2258.3340	Ø 3.3 mm, GH 4.0 mm	67	C2620.4306	Ø 4.3 mm	63
C2258.3825	Ø 3.8 mm, GH 2.5 mm	67	C2620.5006	Ø 5.0 mm	63
C2258.3840	Ø 3.8 mm, GH 4.0 mm	67			
C2258.4325	Ø 4.3 mm, GH 2.5 mm	67		Lab analog	
C2258.4340	Ø 4.3 mm, GH 4.0 mm	67	C3010.3300	Ø 3.3 mm	59
C2258.5035	Ø 5.0 mm, GH 2.5 mm	67	C3010.3800	Ø 3.8 mm	59
C2258.5050	Ø 5.0 mm, GH 4.0 mm	67	C3010.4300	Ø 4.3 mm	59
			C3010.5000	Ø 5.0 mm	59
Bar abutments, 30° angled, type B					
C2259.3325	Ø 3.3 mm, GH 2.5 mm	67		DIM Analog® for the	
C2259.3340	Ø 3.3 mm, GH 4.0 mm	67		CAMLOG® Implant System	
C2259.3825	Ø 3.8 mm, GH 2.5 mm	67	C3012.3300	Ø 3.3 mm	59
C2259.3840	Ø 3.8 mm, GH 4.0 mm	67	C3012.4300	Ø 3.8/4.3 mm	59
C2259.4325	Ø 4.3 mm, GH 2.5 mm	67	C3012.5000	Ø 5.0 mm	59
C2259.4340	Ø 4.3 mm, GH 4.0 mm	67			
C2259.5035	Ø 5.0 mm, GH 2.5 mm	67		Ball abutment analogs	
C2259.5050	Ø 5.0 mm, GH 4.0 mm	67	C3015.3300	Ø 3.3/3.8/4.3 mm	72
			C3015.5000	Ø 5.0 mm	72
Temporary abutment, bridge					
C2339.3300	Ø 3.3 mm	60		Implant analog	
C2339.3800	Ø 3.8 mm	60	C3025.3300	Ø 3.3 mm	59
C2339.4300	Ø 4.3 mm	60	C3025.3800	Ø 3.8 mm	59
C2339.5000	Ø 5.0 mm	60	C3025.4300	Ø 4.3 mm	59
			C3025.5000	Ø 5.0 mm	59
Titanium bases CAD/CAM, bridge					
C2342.3308	Ø 3.3 mm, GH 0.8 mm	62	C3709.0010	Universal holder	82
C2342.3320	Ø 3.3 mm, GH 2.0 mm	62			
C2342.3808	Ø 3.8 mm, GH 0.8 mm	62		Abutment collets	
C2342.3820	Ø 3.8 mm, GH 2.0 mm	62	C3709.3300	Ø 3.3 mm	82
C2342.4308	Ø 4.3 mm, GH 0.8 mm	62	C3709.3800	Ø 3.8 mm	82
C2342.4320	Ø 4.3 mm, GH 2.0 mm	62	C3709.4300	Ø 4.3 mm	82
C2342.5008	Ø 5.0 mm, GH 0.8 mm	62	C3709.5000	Ø 5.0 mm	82
C2342.5020	Ø 5.0 mm, GH 2.0 mm	62			
				Collet for CAM blank, type IAC	
CAM titanium blank, type IAC			C3720.3300	Ø 3.3 mm	64
C2411.3313	Ø 3.3 mm	64	C3720.4300	Ø 3.8/4.3 mm	64
C2411.4313	Ø 3.8/4.3 mm	64	C3720.5000	Ø 5.0 mm	64
C2411.5013	Ø 5.0 mm	64			

C4004.1600	Lab screw with reduced head, hex Ø 3.3/3.8/4.3 mm	70	C8010.1010	SCREW-LINE Macro model	87
C4004.2000	Ø 5.0 mm	70	C8010.1400	PROGRESSIVE-LINE Macro model	87
C4004.1601	Abutment screw with reduced head, hex Ø 3.3/3.8/4.3 mm	70	C8011.1000	Selection abutment kit	83
C4004.2001	Ø 5.0 mm	70		Demonstration model, acrylic glass	
C4005.1601	Abutment screw, hex Ø 3.3/3.8/4.3 mm	77	C8050.1040	Lower jaw	87
C4005.2001	Ø 5.0 mm	77	C8070.1020	Upper jaw	87
C4006.1601	Lab screw, hex Ø 3.3/3.8/4.3 mm	77		Healing cap for bar abutment Ø 3.3/3.8/4.3 mm	68
C4006.2001	Ø 5.0 mm	77	J2029.6000	Ø 5.0 mm	68
C4015.1601	Abutment screw for CONELOG® Titanium bases CAD/CAM Ø 3.3/3.8/4.3 mm	63	J2111.3300	Ø 3.3 mm	58
C4015.2001	Ø 5.0 mm	63	J2111.3800	Ø 3.8 mm	58
			J2111.4300	Ø 4.3 mm	58
			J2111.5000	Ø 5.0 mm	58
C4016.1601	Lab screw for CONELOG® Titanium bases CAD/CAM Ø 3.3/3.8/4.3 mm	63	J2112.3300	Bite registration caps Ø 3.3 mm	59
C4016.2001	Ø 5.0 mm	63	J2112.3800	Ø 3.8 mm	59
			J2112.4300	Ø 4.3 mm	59
			J2112.5000	Ø 5.0 mm	59
C5002.3300	CONELOG® Guiding pin for bone profiler Ø 3.3 mm	43		Impression cap, for bar abutment, closed tray (bridge/bar)	
C5002.3800	Ø 3.8 mm	43	J2129.4300	Ø 3.3/3.8/4.3 mm, short	68
C5002.4300	Ø 4.3 mm	43	J2129.4310	Ø 3.3/3.8/4.3 mm, long	68
C5002.5000	Ø 5.0 mm	43	J2129.6000	Ø 5.0 mm, short	68
			J2129.6010	Ø 5.0/6.0 mm, long	68
C5300.1601	Disconnector Ø 3.3/3.8/4.3 mm, short	81	J2253.0001	Driver for Locator®	79
C5300.1603	Ø 3.3/3.8/4.3 mm, long	81	J2253.0002	Locator® Instrument	79
C5300.2001	Ø 5.0 mm, short	81	J2253.0003	Locator® Angle measurement guide	79
C5300.2003	Ø 5.0 mm, long	81	J2253.0004	Locator® Parallel post	79
C5300.9010	X-Ray Planning foil 1.25:1	16	J2253.0102	Locator® Male processing package	75
C5300.9011	X-Ray Planning foil 1.4:1	16	J2253.0112	Locator® Male processing package for extended range	75
	CONELOG® SCREW-LINE Implants		J2253.0200	Locator® Impression cap	74
C5300.9014	X-Ray Planning foil 1.25:1	16	J2253.0340	Locator® Analog	74
C5300.9015	X-Ray Planning foil 1.4:1	16	J2253.0401	Locator® Block out spacer	75
	CONELOG® PROGRESSIVE-LINE Implants		J2253.0402	Locator® Processing replacement male	75
C5300.9080	X-Ray Transfer pictures 1.25:1 CONELOG® SCREW-LINE Implants Ø 3.3 mm	16		Locator® Replacement male blue	76
C5300.9081	Ø 3.8 mm	16	J2253.1002	pink	76
C5300.9082	Ø 4.3 mm	16	J2253.1003	clear	75
C5300.9083	Ø 5.0 mm	16			
C5302.3310	Adapter for screw implants Ø 3.3 mm, long	47			
C5302.3311	Ø 3.3 mm, short	47			
C5302.4310	Ø 3.8/4.3 mm, long	47			
C5302.4311	Ø 3.8/4.3 mm, short	47			
C5302.5011	Ø 5.0 mm, short	47			

	Locator® Replacement male for extended range		J2552.4300	Logfit® Analog Ø 3.8/4.3 mm	66
J2253.2000	Ø 3.8/4.3/5.0 mm, gray	76	J2552.6000	Ø 5.0 mm	66
J2253.2002	Ø 3.8/4.3/5.0 mm, red	76			
J2253.2003	Ø 3.8/4.3/5.0 mm, orange	76		Logfit® Plastic copings	
J2253.2004	Ø 3.8/4.3/5.0 mm, green	76	J2553.4301	Ø 3.8/4.3 mm, for bridges	66
			J2553.4302	Ø 3.8/4.3 mm, for crowns	66
	Locator® Fixture for bar abutment		J2553.6001	Ø 5.0 mm, for bridges	66
J2253.4301	Ø 3.3/3.8/4.3 mm	70	J2553.6002	Ø 5.0 mm, for crowns	66
J2253.6001	Ø 5.0 mm	70			
				Scanning cap for bar abutments	
	Crown base for bar abutment		J2610.4300	Ø 3.3/3.8/4.3 mm	68
J2256.4306	Ø 3.3/3.8/4.3 mm	69	J2610.6000	Ø 5.0 mm	68
J2256.6006	Ø 5.0 mm	69			
				Bar lab analog for bar abutments	
	Base for bar abutment, burn-out		J3020.4300	Ø 3.3/3.8/4.3 mm	68
J2257.4301	Ø 3.3/3.8/4.3 mm	69	J3020.6000	Ø 5.0 mm	68
J2257.6001	Ø 5.0 mm	69			
				Polishing protection for caps and bases	
	Base for bar abutment, solderable		J3021.4300	Ø 3.3/3.8/4.3 mm	69
J2258.4300	Ø 3.3/3.8/4.3 mm	69	J3021.6000	Ø 5.0 mm	69
J2258.6000	Ø 5.0 mm	69			
				Handle for CAMLOG®/CONELOG® Implant analog	
J2259.4301	Ø 3.3/3.8/4.3 mm, for crown	68	J3025.0010	Ø 3.3/3.8/4.3 mm	81
J2259.4302	Ø 3.3/3.8/4.3 mm, for bridge	69	J3025.0015	Ø 5.0 mm	81
J2259.6001	Ø 5.0 mm, for crown	68			
J2259.6002	Ø 5.0 mm, for bridge	69		Bar implant analog for bar abutments	
			J3025.4300	Ø 3.3/3.8/4.3 mm	68
	Titanium cap without retention for bar abutment, for bridge		J3025.6000	Ø 5.0 mm	68
J2259.4322	Ø 3.3/3.8/4.3 mm	69			
J2259.6022	Ø 5.0 mm	69		Gingiva height indicator, straight	
			J3550.3300	Ø 3.3 mm	68
	Titanium bonding base for bar abutment		J3550.3800	Ø 3.8 mm	68
J2260.4301	Ø 3.3/3.8/4.3 mm	69	J3550.4300	Ø 4.3 mm	68
J2260.6001	Ø 5.0 mm	69	J3550.5000	Ø 5.0 mm	68
			J3551.0001	Orientation gauge for COMFOUR®	68
	Bar sleeve for titanium bonding base				
J2261.4301	Ø 3.3/3.8/4.3 mm	69	J3709.0015	Universal holder	82
J2261.6001	Ø 5.0 mm	69			
				Reworking reamer, for base for bar abutment	
J2262.4300	Ø 3.3/3.8/4.3 mm	69	J3711.0010	Ø 3.3/3.8/4.3 mm, plane surface	82
J2262.6000	Ø 5.0 mm	69	J3711.0015	Ø 5.0 mm, plane surface	82
			J3711.0020	Ø 3.3/3.8/4.3 mm, screw seat	82
	Base for bar abutment, cast-on		J3711.0025	Ø 5.0 mm, screw seat	82
J2263.4300	Ø 3.3/3.8/4.3 mm	69			
J2263.6000	Ø 5.0 mm	69		Guide System seating tool	
J2269.0003	Aligning tool 17°	68	J3716.3300	Ø 3.3 mm	40
J2269.0004	Aligning tool 30°	68	J3716.4300	Ø 3.8/4.3 mm	40
J2269.0005	Aligning tool 17°	68			
J2269.0006	Aligning tool 30°	68		Guide System setting tool PROGRESSIVE-LINE	
			J3717.3300	Ø 3.3 mm	32
	Logfit® Impression caps		J3717.4300	Ø 3.8/4.3 mm	32
J2551.4300	Ø 3.8/4.3 mm	66	J3717.5000	Ø 5.0 mm	32
J2551.6000	Ø 5.0 mm	66			
				Guide System template drill	
			J3733.3300	Ø 3.3 mm	40
			J3733.4300	Ø 3.8/4.3 mm	40

Guide System guiding sleeve			Baring drill for cover screw		
J3734.3303	Ø 3.3 mm	40	J5004.4300	Ø 4.3 mm	43
J3734.3803	Ø 3.8 mm	40	J5004.5000	Ø 5.0 mm	43
J3734.4303	Ø 4.3 mm	40			
Guide System template drill			Countersink		
	PROGRESSIVE-LINE		J5006.3346	Ø 3.3 mm, Ø 4.6 mm	43
J3753.3300	Ø 3.3 mm	32	J5006.3852	Ø 3.8 mm, Ø 5.2 mm	43
J3753.4300	Ø 3.8/4.3 mm	32	J5006.4356	Ø 4.3 mm, Ø 5.6 mm	43
J3753.5000	Ø 5.0 mm	32	J5006.5063	Ø 5.0 mm, Ø 6.3 mm	43
Guide System guiding sleeve			Depth stop SCREW-LINE for pilot drill		
	PROGRESSIVE-LINE			and pre-drill	
J3754.3301	Ø 3.3 mm	32	J5015.0007	L 7 mm	43
J3754.3801	Ø 3.8 mm	32	J5015.0009	L 9 mm	43
J3754.4301	Ø 4.3 mm	32	J5015.0011	L 11 mm	43
J3754.5001	Ø 5.0 mm	32	J5015.0013	L 13 mm	43
Plastic screw for bar abutment			Depth stop for form drill		
J4009.1627	M 1.6	71		PROGRESSIVE-LINE and SCREW-LINE	
J4009.2027	M 2.0	71	J5015.3300	Ø 3.3 mm	23, 37
			J5015.3800	Ø 3.8 mm	23, 37
Prosthetic screw for bar abutments			J5015.4300	Ø 4.3 mm	23, 37
J4012.1601	Ø 3.3/3.8/4.3 mm	70	J5015.5000	Ø 5.0 mm	23, 37
J4012.2001	Ø 5.0 mm	70			
Screw, hex			Guide System gingiva punch		
J4012.1610	L 10 mm, M 1.6	70	J5041.3303	Ø 3.3 mm, SCREW-LINE	39
J4012.1615	L 15 mm, M 1.6	70	J5041.3304	Ø 3.3 mm, PROGRESSIVE-LINE	30
J4012.1620	L 20 mm, M 1.6	70	J5041.3803	Ø 3.8 mm, SCREW-LINE	39
J4012.2010	L 10 mm, M 2.0	70	J5041.3804	Ø 3.8 mm, PROGRESSIVE-LINE	30
J4012.2015	L 15 mm, M 2.0	70	J5041.4303	Ø 4.3 mm, SCREW-LINE	39
J4012.2020	L 20 mm, M 2.0	70	J5041.4304	Ø 4.3 mm, PROGRESSIVE-LINE	30
			J5041.5004	Ø 5.0 mm, PROGRESSIVE-LINE	30
Lab prosthetic screw for bar abutment			J5050.2300	Round bur	42
J4013.1601	Ø 3.3/3.8/4.3 mm	70	J5051.2000	Pilot drill SCREW-LINE	42
J4013.2001	Ø 5.0 mm	70	J5051.2003	Pilot drill	42
Drill extension ISO shaft			J5051.2800	Pre-drill SCREW-LINE	42
J5002.0005	for instruments with internal irrigation	41			
J5002.0006	not for instruments with internal irrigation	44			
J5002.0011	Adapter ISO shaft	46	J5053.3316	Form drill SCREW-LINE Cortical bone	37
J5002.0012	Cleaning needle	48	J5053.3816	Ø 3.3 mm	37
J5002.0013	Wrench adapter	27	J5053.4316	Ø 3.8 mm	37
J5002.0020	Cleaning cannula	48	J5053.5016	Ø 4.3 mm	37
				Ø 5.0 mm	37
Bone profiler			Tap SCREW-LINE		
J5003.3350	Ø 3.3 mm	43	J5054.3309	Ø 3.3 mm	37
J5003.4360	Ø 3.8/4.3 mm	43	J5054.3809	Ø 3.8 mm	37
J5003.5070	Ø 5.0 mm	43	J5054.4309	Ø 4.3 mm	37
			J5054.5009	Ø 5.0 mm	37
Baring drill for cover screw			Form drill SCREW-LINE		
J5004.3300	Ø 3.3 mm	43	J5062.3309	Ø 3.3 mm, L 9	37
J5004.3800	Ø 3.8 mm	43	J5062.3311	Ø 3.3 mm, L 11	37
			J5062.3313	Ø 3.3 mm, L 13	37
			J5062.3316	Ø 3.3 mm, L 16	37
			J5062.3807	Ø 3.8 mm, L 7	37

Form drill SCREW-LINE			Form drill PROGRESSIVE-LINE		
J5062.3809	Ø 3.8 mm, L 9	37	J5070.3309	Ø 3.3 mm, L 9 mm	23
J5062.3811	Ø 3.8 mm, L 11	37	J5070.3311	Ø 3.3 mm, L 11 mm	23
J5062.3813	Ø 3.8 mm, L 13	37	J5070.3313	Ø 3.3 mm, L 13 mm	23
J5062.3816	Ø 3.8 mm, L 16	37	J5070.3316	Ø 3.3 mm, L 16 mm	23
J5062.4307	Ø 4.3 mm, L 7	37	J5070.3807	Ø 3.8 mm, L 7 mm	23
J5062.4309	Ø 4.3 mm, L 9	37	J5070.3809	Ø 3.8 mm, L 9 mm	23
J5062.4311	Ø 4.3 mm, L 11	37	J5070.3811	Ø 3.8 mm, L 11 mm	23
J5062.4313	Ø 4.3 mm, L 13	37	J5070.3813	Ø 3.8 mm, L 13 mm	23
J5062.4316	Ø 4.3 mm, L 16	37	J5070.3816	Ø 3.8 mm, L 16 mm	23
J5062.5007	Ø 5.0 mm, L 7	37	J5070.4307	Ø 4.3 mm, L 7 mm	23
J5062.5009	Ø 5.0 mm, L 9	37	J5070.4309	Ø 4.3 mm, L 9 mm	23
J5062.5011	Ø 5.0 mm, L 11	37	J5070.4311	Ø 4.3 mm, L 11 mm	23
J5062.5013	Ø 5.0 mm, L 13	37	J5070.4313	Ø 4.3 mm, L 13 mm	23
J5062.5016	Ø 5.0 mm, L 16	37	J5070.4316	Ø 4.3 mm, L 16 mm	23
Guide System pilot drill set			J5070.5007	Ø 5.0 mm, L 7 mm	23
J5063.3309	Ø 3.3 mm, L 5/9 mm	38	J5070.5009	Ø 5.0 mm, L 9 mm	23
J5063.3311	Ø 3.3 mm, L 5/9/11 mm	38	J5070.5011	Ø 5.0 mm, L 11 mm	23
J5063.3313	Ø 3.3 mm, L 5/9/13 mm	38	J5070.5013	Ø 5.0 mm, L 13 mm	23
J5063.4307	Ø 3.8/4.3 mm, L 5/7 mm	38	J5070.5016	Ø 5.0 mm, L 16 mm	23
J5063.4309	Ø 3.8/4.3 mm, L 5/9 mm	38	Tap PROGRESSIVE-LINE		
J5063.4311	Ø 3.8/4.3 mm, L 5/9/11 mm	38	J5071.3300	Ø 3.3 mm	23
J5063.4313	Ø 3.8/4.3 mm, L 5/9/11/13 mm	38	J5071.3800	Ø 3.8 mm	23
J5064.3316	Ø 3.3 mm, L 16 mm	38	J5071.4300	Ø 4.3 mm	23
J5064.4316	Ø 3.8/4.3 mm, L 16 mm	38	J5071.5000	Ø 5.0 mm	23
Guide System surgery set, SCREW-LINE			Dense bone drill PROGRESSIVE-LINE		
J5065.3309	Ø 3.3 mm, L 5/9 mm	39	J5072.3300	Ø 3.3 mm	23
J5065.3311	Ø 3.3 mm, L 5/9/11 mm	39	J5072.3800	Ø 3.8 mm	23
J5065.3313	Ø 3.3 mm, L 5/9/11/13 mm	39	J5072.4300	Ø 4.3 mm	23
J5065.3807	Ø 3.8 mm, L 5/7 mm	39	J5072.5000	Ø 5.0 mm	23
J5065.3809	Ø 3.8 mm, L 5/9 mm	39	Guide System pilot drill PROGRESSIVE-LINE		
J5065.3811	Ø 3.8 mm, L 5/9/11 mm	39	J5074.3305	Ø 3.3 mm, L 5 mm	30
J5065.3813	Ø 3.8 mm, L 5/9/11/13 mm	39	J5074.3309	Ø 3.3 mm, L 9 mm	30
J5065.4307	Ø 4.3 mm, L 5/7 mm	39	J5074.3311	Ø 3.3 mm, L 11 mm	30
J5065.4309	Ø 4.3 mm, L 5/9 mm	39	J5074.3313	Ø 3.3 mm, L 13 mm	30
J5065.4311	Ø 4.3 mm, L 5/9/11 mm	39	J5074.3316	Ø 3.3 mm, L 16 mm	30
J5065.4313	Ø 4.3 mm, L 5/9/11/13 mm	39	J5074.4305	Ø 3.8/4.3 mm, L 5 mm	30
J5066.3316	Ø 3.3 mm, L 16 mm	39	J5074.4307	Ø 3.8/4.3 mm, L 7 mm	30
J5066.3816	Ø 3.8 mm, L 16 mm	39	J5074.4309	Ø 3.8/4.3 mm, L 9 mm	30
J5066.4316	Ø 4.3 mm, L 16 mm	39	J5074.4311	Ø 3.8/4.3 mm, L 11 mm	30
Guide System form drill, SCREW-LINE, Cortical Bone			J5074.4313	Ø 3.8/4.3 mm, L 13 mm	30
J5068.3309	Ø 3.3 mm, L 9 mm	39	J5074.4316	Ø 3.8/4.3 mm, L 16 mm	30
J5068.3311	Ø 3.3 mm, L 11 mm	39	J5074.5005	Ø 5.0 mm, L 5 mm	30
J5068.3313	Ø 3.3 mm, L 13 mm	39	J5074.5007	Ø 5.0 mm, L 7 mm	30
J5068.3316	Ø 3.3 mm, L 16 mm	39	J5074.5009	Ø 5.0 mm, L 9 mm	30
J5068.3807	Ø 3.8 mm, L 7 mm	39	J5074.5011	Ø 5.0 mm, L 11 mm	30
J5068.3809	Ø 3.8 mm, L 9 mm	39	J5074.5013	Ø 5.0 mm, L 13 mm	30
J5068.3811	Ø 3.8 mm, L 11 mm	39	J5074.5016	Ø 5.0 mm, L 16 mm	30
J5068.3813	Ø 3.8 mm, L 13 mm	39	Guide System pre-drill PROGRESSIVE-LINE		
J5068.3816	Ø 3.8 mm, L 16 mm	39	J5076.3305	Ø 3.3 mm	31
J5068.4307	Ø 4.3 mm, L 7 mm	39	J5076.3805	Ø 3.8 mm	31
J5068.4309	Ø 4.3 mm, L 9 mm	39	J5076.4305	Ø 4.3 mm	31
J5068.4311	Ø 4.3 mm, L 11 mm	39	J5076.5005	Ø 5.0 mm	31
J5068.4313	Ø 4.3 mm, L 13 mm	39			
J5068.4316	Ø 4.3 mm, L 16 mm	39			

Guide System form drill			Profile drill PROGRESSIVE-LINE Flex		
PROGRESSIVE-LINE			J5080.4300	Ø 4.3 mm	27
J5076.3309	Ø 3.3 mm, L 9 mm	31	J5080.5000	Ø 5.0 mm	27
J5076.3311	Ø 3.3 mm, L 11 mm	31			
J5076.3313	Ø 3.3 mm, L 13 mm	31	J5300.0011	Driver	78
J5076.3316	Ø 3.3 mm, L 16 mm	31	for ball abutment, manual/wrench		
J5076.3807	Ø 3.8 mm, L 7 mm	31			
J5076.3809	Ø 3.8 mm, L 9 mm	31	Driver for straight bar abutment		
J5076.3811	Ø 3.8 mm, L 11 mm	31	J5300.0020	Ø 3.3/3.8/4.3 mm, short	78
J5076.3813	Ø 3.8 mm, L 13 mm	31	J5300.0021	Ø 3.3/3.8/4.3 mm, long	79
J5076.3816	Ø 3.8 mm, L 16 mm	31	J5300.0025	Ø 5.0 mm, short	78
J5076.4307	Ø 4.3 mm, L 7 mm	31			
J5076.4309	Ø 4.3 mm, L 9 mm	31	Removal adapter for		
J5076.4311	Ø 4.3 mm, L 11 mm	31	CAMLOG® and CONELOG®		
J5076.4313	Ø 4.3 mm, L 13 mm	31	J5300.0022	Ø 3.3/3.8/4.3/5.0 mm	23
J5076.4316	Ø 4.3 mm, L 16 mm	31			
J5076.5007	Ø 5.0 mm, L 7 mm	31	Driver for impression cap and		
J5076.5009	Ø 5.0 mm, L 9 mm	31	healing cap for bar abutment		
J5076.5011	Ø 5.0 mm, L 11 mm	31	J5300.0027	Ø 3.3/3.8/4.3 mm	68, 79
J5076.5013	Ø 5.0 mm, L 13 mm	31	J5300.0028	Ø 5.0 mm	68, 79
J5076.5016	Ø 5.0 mm, L 16 mm	31			
Guide System form drill for Ø 3.8 mm			J5300.0030	PickUp instrument	46
under preparation PROGRESSIVE-LINE					
J5077.3309	Ø 3.3 mm, L 9 mm	31	Driver for screw implants		
J5077.3311	Ø 3.3 mm, L 11 mm	31	J5300.0031	extra short, manual/wrench	45
J5077.3313	Ø 3.3 mm, L 13 mm	31	J5300.0032	short, manual/wrench	45
J5077.3316	Ø 3.3 mm, L 16 mm	31	J5300.0033	long, manual/wrench	45
Guide System dense bone drill			with ISO-shaft for angled hand piece		
PROGRESSIVE-LINE			J5300.0034	short (with hexagon at the shaft)	45
J5078.3309	Ø 3.3 mm, L 9 mm	31	J5300.0035	long (with hexagon at the shaft)	45
J5078.3311	Ø 3.3 mm, L 11 mm	31	J5300.0036	short (without hexagon at the shaft)	46
J5078.3313	Ø 3.3 mm, L 13 mm	31	J5300.0037	long (without hexagon at the shaft)	46
J5078.3316	Ø 3.3 mm, L 16 mm	31	J5300.0038	Cardanic driver	46
J5078.3807	Ø 3.8 mm, L 7 mm	31	Surgery set CAMLOG®/CONELOG®		
J5078.3809	Ø 3.8 mm, L 9 mm	31	J5300.0063	SCREW-LINE	36
J5078.3811	Ø 3.8 mm, L 11 mm	31	J5300.0065	PROGRESSIVE-LINE	22
J5078.3813	Ø 3.8 mm, L 13 mm	31	J5300.0071	PROGRESSIVE-LINE Flex	26
J5078.3816	Ø 3.8 mm, L 16 mm	31			
J5078.4307	Ø 4.3 mm, L 7 mm	31	Pattern for surgery wash tray		
J5078.4309	Ø 4.3 mm, L 9 mm	31	CAMLOG®/CONELOG®		
J5078.4311	Ø 4.3 mm, L 11 mm	31	J5300.1068	SCREW-LINE	36
J5078.4313	Ø 4.3 mm, L 13 mm	31	J5300.1070	PROGRESSIVE-LINE	22
J5078.4316	Ø 4.3 mm, L 16 mm	31			
J5078.5007	Ø 5.0 mm, L 7 mm	31	Paralleling pin		
J5078.5009	Ø 5.0 mm, L 9 mm	31	J5300.2000	PROGRESSIVE-LINE	23
J5078.5011	Ø 5.0 mm, L 11 mm	31	J5300.2028	SCREW-LINE	44
J5078.5013	Ø 5.0 mm, L 13 mm	31			
J5078.5016	Ø 5.0 mm, L 16 mm	31	Surgery tray (without content)		
Drill PROGRESSIVE-LINE Flex			CAMLOG®/CONELOG®		
J5079.3300	Ø 3.3 mm	27	J5300.8916	SCREW-LINE	36
J5079.3800	Ø 3.8 mm	27	J5300.8917	PROGRESSIVE-LINE	22
J5079.4300	Ø 4.3 mm	27	J5300.8920	PROGRESSIVE-LINE Flex	26
J5079.5000	Ø 5.0 mm	27			
Profile drill PROGRESSIVE-LINE Flex			Guide System surgery tray		
J5080.3300	Ø 3.3 mm	27	CAMLOG®/CONELOG® (without content)		
J5080.3800	Ø 3.8 mm	27	J5300.8919	PROGRESSIVE-LINE	30

	Surgery wash tray (without content)				
	CAMLOG®/CONELOG®		J5418.5000	Osteotome SCREW-LINE	
J5300.8968	SCREW-LINE	36	J5418.5010	Ø 5.0 mm, straight convex	49
J5300.8970	PROGRESSIVE-LINE	22		Ø 5.0 mm, angled convex	50
	Guide System check-up pin		J5419.2800	Pre-Osteotome SCREW-LINE	
J5301.3300	Ø 3.3 mm, SCREW-LINE	41		1.7 – 2.8 mm, straight concave	51, 52
J5301.3310	Ø 3.3 mm, PROGRESSIVE-LINE	32		Osteotomy set CAMLOG®/	
J5301.4300	Ø 3.8/4.3 mm, SCREW-LINE	41		CONELOG® SCREW-LINE,	
J5301.4310	Ø 3.8/4.3 mm, PROGRESSIVE-LINE	32	J5420.0020	straight concave	51
J5301.5010	Ø 5.0 mm, PROGRESSIVE-LINE	32	J5420.0030	angled concave	52
J5302.0010	Holding key for insertion post	47		Osteotome SCREW-LINE	
	Holding sleeve for screw implants		J5420.3300	Ø 3.3 mm, straight concave	51
J5302.3300	Ø 3.3 mm	47	J5420.3310	Ø 3.3 mm, angled concave	52
J5302.3800	Ø 3.8 mm	47	J5420.3800	Ø 3.8 mm, straight concave	51
J5302.4300	Ø 4.3 mm	47	J5420.3810	Ø 3.8 mm, angled concave	52
J5302.5000	Ø 5.0 mm	47	J5420.4300	Ø 4.3 mm, straight concave	51
	Guide System driver		J5420.4310	Ø 4.3 mm, angled concave	52
J5303.4300	Ø 3.3/3.8/4.3 mm, manual/wrench	41	J5420.5000	Ø 5.0 mm, straight concave	51
J5304.4300	Ø 3.3/3.8/4.3 mm, with ISO shaft	41	J5420.5010	Ø 5.0 mm, angled concave	52
	Screwdriver, hex		J8070.2050	Edentulous mandible	87
J5317.0501	short, manual/wrench	47, 80	M1000.0050	ALTApin magazine, 1 unit	55
J5317.0502	long, manual/wrench	47, 81	M1000.0100	ALTApin magazine, 3 units	55
J5317.0503	long, ISO shaft	48, 81	M5100.0010	ALTApin applicator, straight	53
J5317.0504	short, ISO shaft	48, 81	M5100.0030	ALTApin applicator, angled 90°	53
J5317.0510	extra short, manual/wrench	47, 80	M5100.0050	ALTApin pricker	54
J5317.0511	Manual screwdriver, hex	48, 81	M5100.0070	ALTApin membrane fixator	54
J5320.1030	Torque wrench	78	M5100.0100	ALTApin surgery mallet	54
	Tap adapter		M5200.0010	ALTApin applicator,	
J5322.0010	short	44		straight, work element	53
J5322.0011	long	44	M5200.0055	ALTApin pricker, insert	54
J5330.8500	Prosthetic tray	80	M5500.0050	ALTApin single patient drill, ISO shaft	54
J5330.8600	Prosthetic set	80	M5600.0110	ALTApin set	53
J5330.8700	Prosthetic tray universal	80	M5600.0210	ALTApin tray	53
J5417.2800	Pre-Osteotome SCREW-LINE				
	1.7 – 2.8 mm, straight convex	49, 50			
J5418.0020	Osteotomy set CAMLOG®/				
	CONELOG® SCREW-LINE,				
	straight convex	49			
J5418.0030	angled convex	50			
J5418.3300	Osteotome SCREW-LINE				
	Ø 3.3 mm, straight convex	49			
J5418.3310	Ø 3.3 mm, angled convex	50			
J5418.3800	Ø 3.8 mm, straight convex	49			
J5418.3810	Ø 3.8 mm, angled convex	50			
J5418.4300	Ø 4.3 mm, straight convex	49			
J5418.4310	Ø 4.3 mm, angled convex	50			

Further documentation

Further information on the CONELOG® Products can be found in the following documents:

- CONELOG® Product catalog
- CONELOG® Working instructions
- CONELOG® Instruction for use
- Preparation instructions
- Camlog literature overview
- Camlog and science

The documents are available from the local Camlog representative.

See also:

<https://ifu.camlog.com>

www.camlog.com

References

- [1] Conserva E. Initial stability after placement of a new buttress threaded implant. A case series study. implants. 2019(3): 24-28.
- [2] Rupp J. One-year clinical experience with Progressive-Line implants. EDI journal. 2020(4): 54-63.
- [3] Semper-Hogg W, Kraft S, Stiller S, Mehrhof J, Nelson K. Analytical and experimental position stability of the abutment in different dental implant systems with a conical implant-abutment connection. Clin Oral Investig 2010;17(3): 1017-23.
- [4] Semper Hogg W, Zulauf K, Mehrhof J, Nelson K. The influence of torque tightening on the position stability of the abutment in conical implant-abutment connections. Int J Prosthodont 2015;28: 538-41.

Trademarks and copyright

Protected trade names (trademarks) are not always specially indicated. The absence of such an indication does not mean that this name is NOT a trademark. The document including all its parts is protected by copyright. You may download the content regarding the intended use, but changes to or reproduction of the content are not permitted. Any exploitation beyond the narrow limits of the copyright act is not permitted without prior written approval of CAMLOG Biotechnologies GmbH and is subject to legal sanctions.

CE0123

Art. No. J8001.0009 Rev. 07 07/2021



Headquarters

CAMLOG Biotechnologies GmbH | Margarethenstr. 38 | 4053 Basel | Switzerland
Phone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.camlog.com

Manufacturer CAMLOG® and CONELOG® Products: ALTATEC GmbH | Maybachstr. 5 | 71299 Wimsheim | Germany

